

# Sterilization effect of atmospheric pressure non-thermal air plasma on dental instruments

Su-Jin Sung<sup>1</sup>, DDS, MSD, Jung-Bo Huh<sup>1</sup>, DDS, MSD, PhD, Mi-Jung Yun<sup>1</sup>, DDS, MSD, PhD, Brian Myung W. Chang<sup>2</sup>, DDS, FACP, FAAMP, Chang-Mo Jeong<sup>1</sup>, DDS, MSD, PhD, Young-Chan Jeon<sup>1\*</sup>, DDS, MSD, PhD

<sup>1</sup>Department of Prosthodontics, School of Dentistry, Pusan National University, Yangsan, Republic of Korea

<sup>2</sup>Department of Maxillofacial Prosthodontics, Cleveland Clinic, Head and Neck Institute, Cleveland, Ohio, USA

**PURPOSE.** Autoclaves and UV sterilizers have been commonly used to prevent cross-infections between dental patients and dental instruments or materials contaminated by saliva and blood. To develop a dental sterilizer which can sterilize most materials, such as metals, rubbers, and plastics, the sterilization effect of an atmospheric pressure non-thermal air plasma device was evaluated. **MATERIALS AND METHODS.** After inoculating *E. coli* and *B. subtilis* the diamond burs and polyvinyl siloxane materials were sterilized by exposing them to the plasma for different lengths of time (30, 60, 90, 120, 180 and, 240 seconds). The diamond burs and polyvinyl siloxane materials were immersed in PBS solutions, cultured on agar plates and quantified by counting the colony forming units. The data were analyzed using one-way ANOVA and significance was assessed by the LSD *post hoc* test ( $\alpha=0.05$ ). **RESULTS.** The device was effective in killing *E. coli* contained in the plasma device compared with the UV sterilizer. The atmospheric pressure non-thermal air plasma device contributed greatly to the sterilization of diamond burs and polyvinyl siloxane materials inoculated with *E. coli* and *B. subtilis*. Diamond burs and polyvinyl siloxane materials inoculated with *E. coli* was effective after 60 and 90 seconds. The diamond burs and polyvinyl siloxane materials inoculated with *B. subtilis* was effective after 120 and 180 seconds. **CONCLUSION.** The atmospheric pressure non-thermal air plasma device was effective in killing both *E. coli* and *B. subtilis*, and was more effective in killing *E. coli* than the UV sterilizer. [J Adv Prosthodont 2013;5:2-8]

**KEY WORDS:** Sterilization; Cross Infections; Non-thermal Atmospheric Pressure Plasma; Bacteria

## INTRODUCTION

Dental treatments can frequently induce cross-contamination between dental patients and dentists through instruments and materials as well as between impression materi-

als and dental technicians.<sup>1-6</sup> Dentists and their assistants should consider a counterplan to protect themselves from pathogenic microorganisms when they treat dental patients with such microorganisms.<sup>1,2,7</sup>

Generally, dental materials made of metal can be disinfected by autoclave sterilization, whereas rubbers or plastics can be sterilized by either chemical methods using glutaldehyde or physical methods using ultrasound and ultraviolet.<sup>8</sup> Autoclave sterilization is specified by medical procedural law as being effective in the prevention of cross-contamination by removing and destroying pathogens.<sup>9</sup> However, the wet technique can reduce the durability of instruments by corroding their surfaces, while the dry technique requires more time for sterilization and can blunt knife edges.<sup>8,10</sup> Ethylene oxide sterilizers, which are generally used in hospitals where many surgeries are performed, have the drawbacks of being impractical in terms of size, price and safety in clinical practice.<sup>8,10,11</sup> The sterilization efficacy of autoclaving is well verified. However,

Corresponding author:  
Young-Chan Jeon  
Department of Prosthodontics, School of Dentistry, Pusan National University, Beom-eo li, Mul-geumeup, Yangsan, 626-870, Republic of Korea  
Tel. 82553605130; e-mail, jeonyc@paran.com  
Received September 27, 2012 / Last Revision December 27, 2012 / Accepted February 8, 2013

© 2013 The Korean Academy of Prosthodontics  
This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

This work was supported by a 2-Year Research Grant of Pusan National University.

to prepare dental instruments for individual dental patients, dentists should possess a corresponding number of instruments, such as high-speed and low-speed hand pieces attached to the dental treatment unit. Dentists face problems of reduction in performance and durability of the instruments due to repeated autoclave sterilization.<sup>8,10</sup> Thus, the necessity for new sterilization devices that are acceptably safe, efficient and economically feasible has been proposed.<sup>7</sup> Moisan *et al.* applied plasma which was produced at low-pressure to *B. subtilis* and chemical radicals such as oxygen atom or excited oxygen molecules appeared to contribute to sterilization. Moreover, numbers of studies have shown the characteristic of plasma that deactivates microorganism including spores, gram negative and positive bacteria, yeast, and virus. Since such low-pressure plasma was being produced in vacuum state, complex and costly equipment was required. However, there has been development of technology which enables the production of stable and non-thermal plasma under atmospheric pressure. The atmospheric plasma can produce numbers of chemical substances constantly, has no toxicity, and is a new biomedical application and method at a low cost. Recent interest has been focused on the studies of interactions between non-thermal plasma and viable

tissues, as well as their applications in the medical field.<sup>12-14</sup> In clinical practice, we could potentially use sterilization devices utilizing the plasma principle to remove toxic materials from surfaces<sup>7,11,15</sup> and tooth bleaching techniques using non-thermal atmospheric pressure plasma.<sup>16</sup>

This study was conducted to verify the sterilization efficacy and safety of a non-thermal atmospheric pressure air plasma device.

## MATERIALS AND METHODS

The assessment for the sterilization efficacies of an atmospheric pressure non-thermal air plasma device which was specially designed for this experiment (Fig. 1) and an ultraviolet (UV) sterilizer (Dentistar SHIELD, Hallim Dentech, Japan) (Fig. 2) in decontaminating dental instruments was performed. Table 1 and 2 show the dimensions of each instrument.

The experimental materials were diamond burs (EX-26, Mani Inc., Japan) and silicon impression materials (Imprint, 3M ESPE, USA) (Fig. 3). Each silicon impression specimen was cut into a regular hexahedron of 10 × 10 × 10 mm, whose one surface was roughened using 100-grit SiC paper for the inoculation of bacterial suspen-

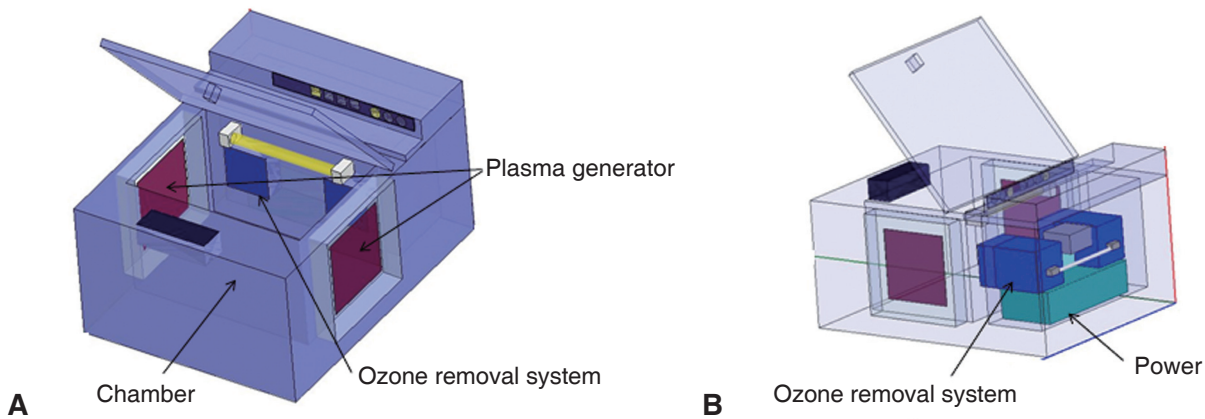


Fig. 1. Schematic view of an atmospheric pressure non-thermal air plasma device. A: The frontal view, B: The rear view.

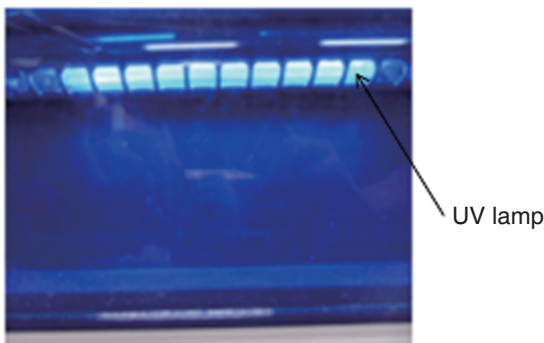


Fig. 2. Schematic view of a UV sterilizer.

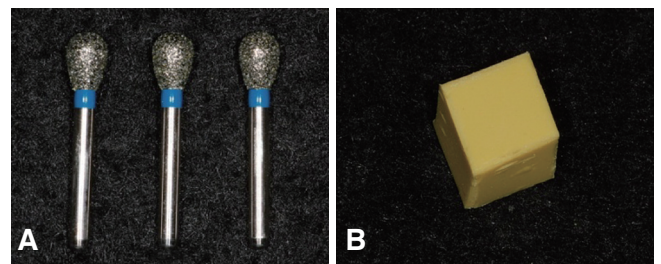


Fig. 3. Inoculated material. A: Diamond bur, B: Polyvinyl siloxane.

**Table 1.** Specification of experimental atmospheric pressure non-thermal air plasma device

Component	Specifications
Chamber	W × D × H: 130 × 130 × 80 mm W × D: 40 × 60 mm
Plasma generator	Sandwich electrode (copper sheet, glass plate, stainless steel mesh)
Ozone removal system	Air pump, Activated carbon, Manganese dioxide
Power	LF power module, 6 kV, 20 kHz

**Table 2.** Specification of UV sterilizer

Component	Specifications
Chamber	W × D × H: 320 × 85 × 110 mm
UV Lamp	Wave length: 253.7 nm
Power	220 V, 50/60 Hz

sions. Each of the diamond burs and silicon impression specimens was immersed in 7% ethanol solution before inoculation with bacterial suspension.

Gram-negative *Escherichia coli* (*E. coli*, KCTC1611) and gram-positive *Bacillus subtilis* (*B. subtilis*, KCTC 1396) were used for this study. *E. coli* was cultured in Luria-Bertani media (1% sodium chloride, 0.5% yeast extract and 1% tryptone) at 37°C at 200 rpm. *B. subtilis* was cultured in nutrient broth (0.5% peptone and 0.3% beef extract) in the same manner as described above.

After the diamond burs and silicone impression materials were inoculated using micropipettes within the testing bench with 5 and 10 µL of *E. coli* suspension, respectively, they were sterilized with the plasma device for 30, 60, 90 and 120 seconds. The same procedures were performed using the *B. subtilis* suspension for 60, 120, 180 and 240 seconds. Each specimen was immersed in a phosphate-buffered saline (PBS) solution. The PBS solution containing surviving bacteria was diluted at 1,000 times and was smeared on an agar plate. The plate was

**Table 3.** Performance tests

	Material	Sterilization device	
		Plasma	UV
<i>E. coli</i>	Diamond bur	30, 60, 90, 120 s	120 s
	Polyvinyl siloxane	30, 60, 90, 120 s	-
<i>B. subtilis</i>	Diamond bur	30, 60, 120, 180 s	-
	Polyvinyl siloxane	60, 120, 180, 240 s	-

cultured at 37°C for 15 hours in a CO<sub>2</sub> incubator (Forma Scientific, International MI/SS Inc, USA) The colony-forming units (CFU) of the cultured bacteria were counted. Sterilization efficacy was assessed by CFU per the unit volume of the PBS. Each experiment at each time point was repeated 4 times (Table 3).

The *E. coli* suspension and the diamond burs were used for these comparisons. They were sterilized using the plasma device and the UV sterilizer. Sterilization efficacy of these 2 sterilizers was assessed in the same manner as mentioned above (Table 3).

Statistical analyses were performed using the SPSS statistical package program (Release 12.0, SPSS Inc, Chicago, IL, USA). The sterilization efficacy of the atmospheric pressure non-thermal air plasma device was examined by one-way ANOVA, and significance was assessed by the LSD post hoc test at  $P < .05$  level of significance. Comparisons of sterilization efficacy between the 2 sterilizers were made using the paired t test.

## RESULTS

Table 4 presents the results of the *E. coli* cultures. The CFU for *E. coli* was greater than 10<sup>9</sup>/mL before plasma sterilization, which was decreased after plasma sterilization. Table 4 shows the logarithms of the mean ( $\pm$  standard deviation) CFU values in order to examine sterilization efficacy against the *E. coli* suspension at different time points. CFU was significantly decreased from second 60 onward ( $P < .05$ ) (Table 5). The logarithmic sterilization efficacy curves are shown in Fig. 4.

**Table 4.** Mean values and standard deviations of *E. coli* surviving (CFU/mL) after treatment with an atmospheric pressure non-thermal air plasma device

Material	Treatment time				
	0 s	30 s	60 s	90 s	120 s
Diamond bur	4.57 × 10 <sup>9</sup>	9.15 × 10 <sup>8</sup>	1.74 × 10 <sup>8</sup>	1.03 × 10 <sup>6</sup>	7.50 × 10 <sup>3</sup>
	(2.59 × 10 <sup>9</sup> )	(2.59 × 10 <sup>8</sup> )	(7.64 × 10 <sup>7</sup> )	(7.30 × 10 <sup>5</sup> )	(1.44 × 10 <sup>3</sup> )
Polyvinyl siloxane	3.45 × 10 <sup>9</sup>	2.75 × 10 <sup>9</sup>	2.37 × 10 <sup>9</sup>	7.61 × 10 <sup>8</sup>	9.86 × 10 <sup>6</sup>
	(1.51 × 10 <sup>9</sup> )	(1.29 × 10 <sup>9</sup> )	(1.40 × 10 <sup>9</sup> )	(4.28 × 10 <sup>8</sup> )	(5.15 × 10 <sup>6</sup> )


Numbers in parentheses are standard deviations.

Table 6 shows the mean ( $\pm$  standard deviation) of CFU for *B. subtilis* at the different time points. The CFU was decreased after plasma sterilization.


Table 7 shows the logarithms of the means ( $\pm$  standard deviation) of the CFU values in order to examine sterilization efficacy at different time points. CFU was significantly decreased from second 120 onward for diamond burs ( $P < .05$ ), which was significantly decreased from second 180 onward for silicone impression materials ( $P < .05$ ) (Table 8). Fig. 5 depicts logarithmic CFU curves

for sterilization efficacy.

The means ( $\pm$  standard deviation) of CFU for *E. coli* obtained 120 seconds after the UV and plasma sterilization are shown in Table 8. The logarithms of the means ( $\pm$  standard deviation) of the CFU values are shown in Table 9. There were significant differences in sterilization efficacy between the 2 sterilizers ( $P < .05$ ) (Table 9). The CFU value was significantly lower in the atmospheric pressure non-thermal air plasma device than in the UV sterilizer.

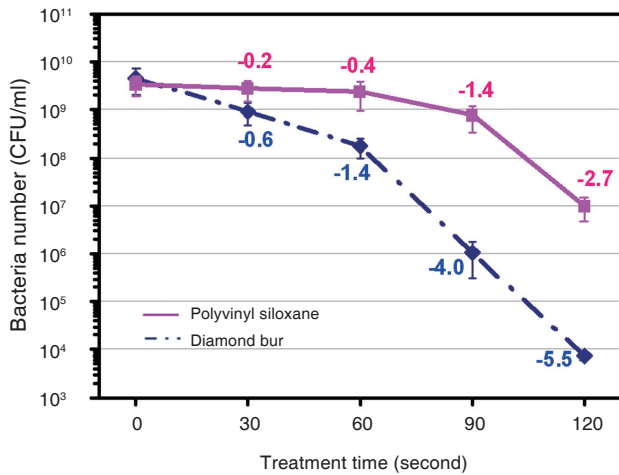

**Fig. 4.** Survival curve (CFU/mL) of *E. coli* after treatment with an atmospheric pressure non-thermal air plasma device as a function of treatment time.

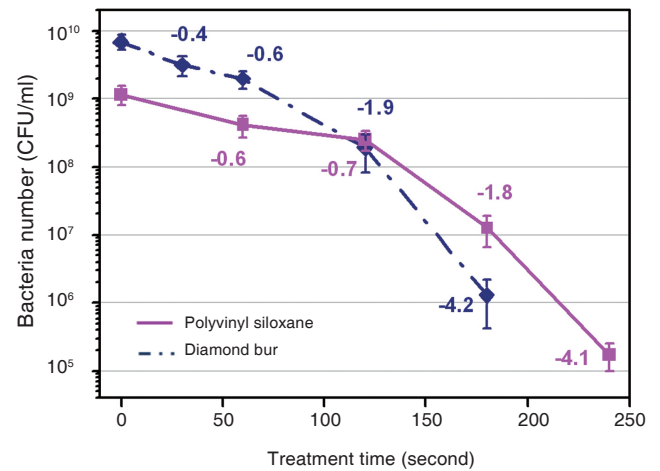

**Fig. 5.** Survival curve (CFU/mL) of *B. subtilis* after treatment with an atmospheric pressure non-thermal air plasma device as a function of treatment time.

**Table 5.** Mean values and standard deviations of *E. coli* surviving on diamond bur and polyvinyl siloxane after treatment with an atmospheric pressure non-thermal air plasma device (LogN/N0)

Material	Treatment time				
	0 s	30 s	60 s	90 s	120 s
Diamond bur	0	$-0.56 \pm 0.18^a$	$-1.41 \pm 0.24^b$	$-4.01 \pm 1.35^c$	$-5.53 \pm 0.70^d$
Polyvinyl siloxane	0	$-0.19 \pm 0.21^A$	$-0.40 \pm 0.30^A$	$-1.39 \pm 1.36^B$	$-2.73 \pm 0.99^C$

**Table 6.** Mean values and standard deviations of *B. subtilis* surviving (CFU/mL) after treatment with an atmospheric pressure non-thermal air plasma device

Material	Treatment time					
	0 s	30 s	60 s	120 s	180 s	240 s
Diamond bur	$6.87 \times 10^9$ ( $1.63 \times 10^9$ )	$3.17 \times 10^9$ ( $1.01 \times 10^9$ )	$1.97 \times 10^9$ ( $5.66 \times 10^8$ )	$1.90 \times 10^8$ ( $1.06 \times 10^8$ )	$1.29 \times 10^6$ ( $8.62 \times 10^5$ )	-
Polyvinyl siloxane	$1.16 \times 10^9$ ( $3.44 \times 10^8$ )	-	$4.19 \times 10^8$ ( $1.46 \times 10^7$ )	$2.54 \times 10^8$ ( $8.36 \times 10^7$ )	$1.29 \times 10^7$ ( $6.30 \times 10^6$ )	$1.75 \times 10^5$ ( $7.51 \times 10^4$ )

Numbers in parentheses are standard deviations.

**Table 7.** Mean values and standard deviations of *B. subtilis* surviving on diamond bur and polyvinyl siloxane after treatment with an atmospheric pressure non-thermal air plasma device (LogN/N0)

Material	Treatment time					
	0 s	30 s	60 s	120 s	180 s	240 s
Diamond bur	0	-0.38 ± 0.14 <sup>a</sup>	-0.57 ± 0.22 <sup>a</sup>	-1.95 ± 0.85 <sup>b</sup>	-4.28 ± 0.67 <sup>c</sup>	-
Polyvinyl siloxane	0	-	-0.56 ± 0.13 <sup>A</sup>	-0.68 ± 0.05 <sup>A</sup>	-1.80 ± 1.53 <sup>B</sup>	-4.12 ± 0.30 <sup>C</sup>

Identical superscripted letters indicate that values are not significantly different ( $P > .05$ ).

**Table 8.** Mean values and standard deviations of *E. coli* surviving (CFU/mL) after treatment with an atmospheric pressure non-thermal air plasma device and UV sterilizer on diamond burs

Sterilization device	Treatment time	
	0 s	120 s
Plasma		9.25 × 10 <sup>4</sup> (7.25 × 10 <sup>4</sup> )
UV	8.60 × 10 <sup>8</sup>	1.69 × 10 <sup>8</sup> (3.07 × 10 <sup>7</sup> )

Numbers in parentheses are standard deviations.

**Table 9.** Mean values and standard deviations of *E. coli* surviving after treatment with an atmospheric pressure non-thermal air plasma device and UV sterilizer on diamond burs (LogN/N0)

Sterilization device	Mean	SD	T	P
Plasma	-4.34	0.60	-15.606	.001
UV	-0.73	0.14		

## DISCUSSION

Infectious diseases, such as hepatitis B, hepatitis C and tuberculosis, can be transmitted to other dental patients or dental professionals during dental treatment through either direct contact with blood and saliva of patients or through indirect contact with contaminated instruments.<sup>2,8,17</sup> For this reason, it is important to prevent cross-contamination between dental patients and dental professionals.<sup>1,8,18</sup>

The importance of infection control at dental clinics has been recognized since the actual state of infections at dental clinics was broadcast through mass media.<sup>1</sup> Consequently, the Korean Ministry of Health and Welfare has prepared the criteria for dental infection control during dental treatment and has established a legislation for the disinfection and sterilization of dental instruments and materials.<sup>9</sup> The term “disinfection” means reduction in the number of pathogenic microorganisms excluding spores, while the term “sterilization” means reduction in the number of pathogenic microorganisms including spores.<sup>8,9</sup> Liquid chemicals are commonly used for disinfection, but ultrasound and UV light are sometimes used. Sterilization methods include autoclaving, gas, dry heat, hydrogen peroxide gas plasma and liquid chemical sterilizations.<sup>9,14,15,19</sup> Because inadequate disinfection and sterilization are the main causes of infections at dental clinics, dental instruments and materials should be completely disinfected or sterilized to prevent cross-contamination at dental clinics.

The autoclaving and dry heat sterilization methods are difficult to use for heat-labile instruments, while the low-temperature gas sterilization method raises problems of safety and expense.<sup>15,19</sup> In addition, since these methods require given time intervals, rapid sterilization is difficult to perform. Although sterilization methods using  $r$ -rays, electronic beams and UV light have been proposed, these methods have some limitations due to inadequate performance, instability and high costs. Thus, further studies on new sterilization methods are warranted. There have been numerous studies on non-thermal plasma sterilization at room temperature.<sup>11,14,20,21</sup> The mechanisms by which the non-thermal plasma device inactivate bacteria have been suggested.<sup>15,22</sup> Plasma is a state in which all materials are completely ionized.<sup>10</sup> Abundant ions, free radicals and UV light generated by non-thermal plasma have various effects: killing cancer cells, tooth bleaching, hemostasis and the eradication of microorganisms.<sup>19</sup> Laroussi<sup>23</sup> have also reported that factors inactivating microorganisms, which are generated by non-thermal plasma, include free radicals, charged particles and UV light. Non-thermal plasma was initially synthesized in a vacuum condition. However, as the problems with inhomogeneity and instability of electric discharge have been solved, atmospheric pressure non-thermal air plasma technologies have been applied to the disinfection and sterilization of dental instruments.<sup>10,20,22</sup>

*E. coli* and *B. subtilis* have frequently been used in previous experimental studies and thus were chosen for this study.<sup>15,17</sup> *E. coli* is a pathogen related to focal or systemic



infections, is easily cultured as a gram-negative rod and has a significant resistance to various external factors.<sup>15,17</sup> *B. subtilis* is a spore-forming gram-positive rod, has a higher resistance to sterilization than gram-negative bacteria and is currently used as a biological indicator of sterilization efficacy.<sup>8,20</sup> Dental burs and silicone impression materials are often contaminated with the blood and saliva of dental patients during treatment.<sup>6</sup> Thus, these burs and materials were chosen for this study. The atmospheric pressure non-thermal air plasma device decreased the CFUs for both *E. coli* and *B. subtilis* (Tables 4 and 6). The procedure significantly decreased CFU in the diamond burs from second 60 onward for *E. coli* (Table 5) and from second 120 onward for *B. subtilis* (Table 7). In the silicone impression materials, the CFU was significantly decreased from second 90 onward for *E. coli* (Table 5) and from second 180 onward for *B. subtilis* (Table 7). In general, *E. coli* showed quicker reductions in CFU than *B. subtilis*. The atmospheric pressure non-thermal air plasma showed better sterilization rates than the UV sterilizer (Tables 8 and 9). The UV sterilizer had sterilization efficacy only in its contact areas, whereas the non-thermal air plasma was effective in all areas in contact with the air due to the dispersion of the plasma through the air.<sup>7</sup> The plasma device contained oxygen free radicals, hydroxyl free radicals, hydrogen peroxide and ozone. Among them, ozone has both a high sterilization efficacy and a potent oxidizing activity.<sup>24</sup> A maximum ozone concentration of 0.1 ppm is allowed in workplaces.<sup>7</sup> To remove ozone from the plasma device, activated charcoal and manganese dioxide was passed through the plasma device using an air pump.<sup>7</sup> Three minutes after the use of the air pump, the ozone concentration reached the values of  $\leq 0.025$  ppm and thus the effect of ozone was excluded from our experiment results.

This study has some limitations. First, a complete sterilization efficacy of the plasma device was observed but was not obtained in this study. Further studies on this issue are required. Second, there are numerous pathogens other than *E. coli* and *B. subtilis*, including Streptococcus mutans (a cariogenic flora), Candida albicans (a causative agent of denture stomatitis) and hepatitis B virus (which 10% of the dentists are infected by).<sup>4,5</sup> More research on these causative microorganisms is needed to support our results. In addition, a detailed mechanism for the effects of plasma on sterilization efficacy remains to be elucidated.

## CONCLUSION

In the diamond burs and silicone impression materials, the CFU was significantly reduced for both *E. coli* and *B. subtilis* after treatment with atmospheric pressure non-thermal air plasma. The CFU was also more significantly reduced for *E. coli* by the atmospheric pressure non-thermal air plasma device than by the UV sterilizer. The results of this study provide the basis for the development of a new simpler, cheaper and more convenient

atmospheric pressure non-thermal air plasma device for clinical practice.

## REFERENCES

1. Choi HN, Bae HS, Cho YS. Literature review of dental infection control in Korea. J Dent Hyg Sci 2010;10:199-209.
2. Hutchings ML, Vandewalle KS, Schwartz RS, Charlton DG. Immersion disinfection of irreversible hydrocolloid impressions in pH-adjusted sodium hypochlorite. Part 2: Effect on gypsum casts. Int J Prosthodont 1996;9:223-9.
3. Leung RL, Schonfeld SE. Gypsum casts as a potential source of microbial cross-contamination. J Prosthet Dent 1983;49:210-1.
4. McNeill MR, Coulter WA, Hussey DL. Disinfection of irreversible hydrocolloid impressions: a comparative study. Int J Prosthodont 1992;5:563-7.
5. Runnells RR. An overview of infection control in dental practice. J Prosthet Dent 1988;59:625-9.
6. Jennings KJ, Samaranyake LP. The persistence of microorganisms on impression materials following disinfection. Int J Prosthodont 1991;4:382-7.
7. Morfill GE, Shimizu T, Steffes B, Schmidt HU. Nosocomial infections-a new approach towards preventive medicine using plasmas. New J phys 2009;11:115019.
8. Samaranyake L. Essential Microbiology for dentistry. 3<sup>rd</sup> ed. Churchill Livingstone; 2007. p. 385-412.
9. Guideline of sterilization of appliance and article at medical institution. Ministry of Health and Welfare Notification No. 2010-61, 2010. 8. 13 enactment
10. Moreau M, Orange N, Feuilleley MG. Non-thermal plasma technologies: new tools for bio-decontamination. Biotechnol Adv 2008;26:610-7.
11. Lee K, Paek KH, Ju WT, Lee Y. Sterilization of bacteria, yeast, and bacterial endospores by atmospheric-pressure cold plasma using helium and oxygen. J Microbiol 2006;44:269-75.
12. Dobrynin D, Fridman G, Friedman G, Fridman A. Physical and biological mechanisms of direct plasma interaction with living tissue. New J Phys 2009;11:115020.
13. Fridman G, Friedman G, Gutsol A, Shekhter AB, Vasilets VN, Fridman A. Applied plasma Medicine. Plasma Process Polym 2008;5:503-33.
14. McCombs GB, Darby ML. New discoveries and directions for medical, dental and dental hygiene research: low temperature atmospheric pressure plasma. Int J Dent Hyg 2010;8:10-5.
15. Sladek REJ, Stoffels E. Deactivation of Escherichia coli by the plasma needle. J Phys D Appl Phys 2005;38:1716-21.
16. Lee HW, Kim GJ, Kim JM, Park JK, Lee JK, Kim GC. Tooth bleaching with nonthermal atmospheric pressure plasma. J Endod 2009;35:587-91.
17. Samaranyake LP, Hunjan M, Jennings KJ. Carriage of oral flora on irreversible hydrocolloid and elastomeric impression materials. J Prosthet Dent 1991;65:244-9.
18. Smith A, Creanor S, Hurrell D, Bagg J, McCowan M. Management of infection control in dental practice. J Hosp

- Infect 2009;71:353-8.
19. Seo YS, Mohamed AAH, Woo KC, Lee HW, Lee JK, Kim KT. Comparative studies of atmospheric pressure plasma characteristics between He and Ar working gases for sterilization. *IEEE Trans Plasma Sci IEEE Nucl Plasm* 2010;38:1954-62.
  20. Iza F, Kim GJ, Lee SM, Lee JK, Walsh JL, Zhang YT, Kong MG. Microplasmas: Sources, particle kinetics, and biomedical applications. *Plasma Process Polym* 2008;5:322-44.
  21. Laroussi M. Low Temperature Plasma-Based Sterilization: Overview and state-of-the Art. *Plasma Process Polym* 2005;2:391-400.
  22. Fridman G, Brooks AD, Balasubramanian M, Fridman A, Gutsol A, Vasilets VN, Ayan H, Friedman G. Comparison of direct and indirect effects of non-thermal atmospheric-pressure plasma on bacteria. *Plasma Process Polym* 2007;4:370-5.
  23. Laroussi M. Nonthermal decontamination of biological media by atmospheric-pressure plasma: review, analysis, and prospects. *IEEE Trans Plasma Sci* 2002;30:1409-15.
  24. Suzuki T, Oizumi M, Furuya J, Okamoto Y, Rosenstiel SF. Influence of ozone on oxidation of dental alloys. *Int J Prosthodont* 1999;12:179-83.