

# Effect of changing the kilovoltage peak on radiographic caries assessment in digital and conventional radiography

Mohamed Khalifa Zayet<sup>1,\*</sup>, Yara Rabee Helaly<sup>1</sup>, Salma Belal Eiid<sup>1</sup>

<sup>1</sup>Oral Radiology Department, Faculty of Oral and Dental Medicine, Cairo University, Egypt

## ABSTRACT

**Purpose:** This study aimed to investigate the effect of changing the kilovoltage peak (kVp) on the radiographic assessment of dental caries.

**Materials and Methods:** Seventy-five extracted posterior teeth with proximal caries or apparently sound proximal surfaces were radiographed with conventional E-speed films and a photostimable phosphor system using 60 kVp and 70 kVp for the caries assessment. The images were evaluated by three oral radiologists and compared with the results of the stereomicroscope analysis.

**Results:** No statistically significant difference was found between 60 kVp and 70 kVp for the caries detection, determination of caries extension into dentin, and caries severity in either the conventional or the digital images. Good to very good inter-observer and intra-observer agreements were found for both kilovoltage values on the conventional and digital images.

**Conclusion:** Changing the kilovoltage between 60 kVp and 70 kVp had no obvious effect on the detection of proximal caries or determination of its extension or severity. (*Imaging Sci Dent* 2014; 44: 199-205)

**KEY WORDS:** Diagnosis, Oral; Dental Caries; Digital Radiography, Dental; Radiography, Dental

## Introduction

Early diagnosis of primary dental caries and limitation of its harmful effects is the first concern in epidemiological studies.<sup>1-4</sup> In daily clinical work, if we exclude sophisticated new methods, radiographic examination is the most frequently recommended method as a supplement to clinical inspection in the assessment of carious lesions.<sup>5,6</sup> This recommendation is particularly emphasized in the assessment of proximal caries.<sup>7</sup>

Although digital radiography has replaced conventional (film-based) radiography to a varying extent in the developed and the developing countries due to its advantages,<sup>8-11</sup> the degree of accuracy of both techniques in caries assess-

ment is not consistent; one of them was considered superior in some studies,<sup>12-15</sup> but other researchers believed that there was no significant difference between conventional and digital radiography with respect to caries assessment.<sup>16-20</sup>

Radiographic assessment of dental caries depends to a large extent on the visual and geometric characteristics of the image. One of these visual characteristics is image contrast.<sup>21</sup> Tube voltage (kilovoltage peak; kVp) is the main factor affecting the image contrast; low kVp provides a short-grayscale and high-contrast image, while increasing kVp is indicated when a long-grayscale and low-contrast image is required.<sup>22,23</sup>

“A radiograph with a high contrast is useful for the detection and progression of dental caries.”; “Some dentists prefer radiographs with a short-grayscale contrast, thinking that dental caries is easier to recognize.”: These statements are part of oral radiology textbooks.<sup>24-27</sup> It is important to determine whether this assumption is still valid and

Received January 14, 2014; Revised February 26, 2014; Accepted April 15, 2014

\*Correspondence to : Dr. Mohamed Khalifa Zayet


Oral Radiology Department, Faculty of Oral and Dental Medicine, Cairo University, 11, El-Saraya St. Al-Manyal, Cairo 11553, Egypt

Tel) 20-100-564-5900, Fax) 20-2-2364-6375, E-mail) m\_khalifa\_z@yahoo.com

Copyright © 2014 by Korean Academy of Oral and Maxillofacial Radiology

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

Imaging Science in Dentistry · pISSN 2233-7822 eISSN 2233-7830

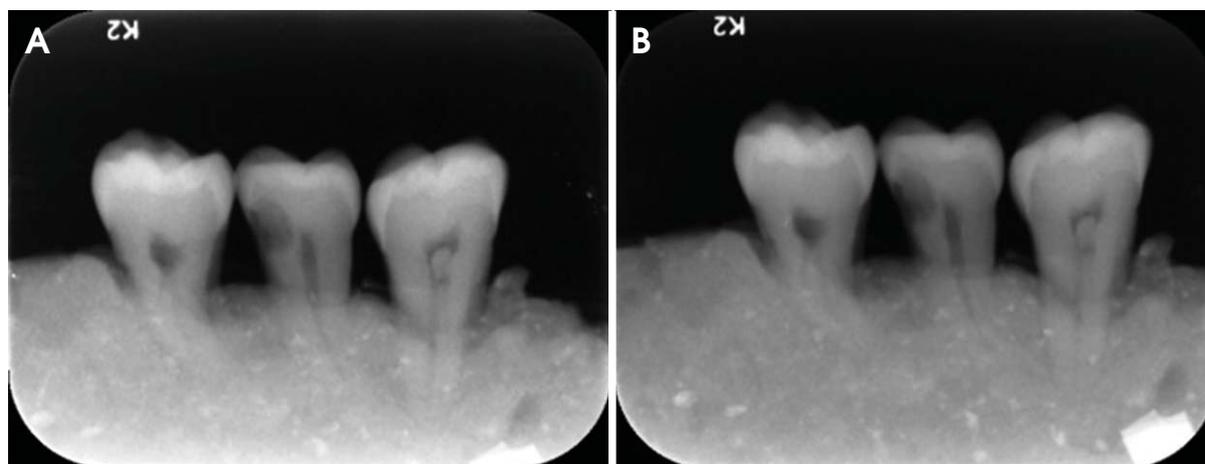

**Fig. 1.** Digital radiographic images show the teeth radiographed with 60 kVp (A) and 70 kVp (B).

whether this validity is equal for digital images and conventional radiographs.

The aim of this study was to investigate the effect of changing tube voltage on caries assessment based on digital and conventional radiographs.

### Materials and Methods

This study was conducted on 150 proximal surfaces of 75 human posterior teeth that were extracted for periodontal or orthodontic reasons. The selected teeth were visually sound or with proximal caries without occlusal cavitation and without extended buccal or lingual/palatal caries. Sets of three teeth each were mounted in contact in a mold made of plaster of Paris (Gipsina, Giza, Egypt). The level of gypsum was adjusted to be below the cemento-enamel junction of the examined teeth by 1-3 mm. A small piece of lead foil was attached to the tube side of the mold to indicate the mesial side of each image. All teeth were radiographed twice by using an intraoral X-ray machine (Minray, Soredex, Tuusula, Finland) set once at 60 kVp and the other time at 70 kVp. The tube current was 7 mA. The focus-to-film distance as well as the tube angulation between the central rays and the image receptors was fixed by using a simple cylindrical device. Eight 1.5-mm-thick layers of pink wax, leading to a total thickness of 12 mm, were placed between the position-indicating device (PID) and the teeth to simulate the effect of soft tissues in the oral cavity.<sup>28</sup> Two types of image receptors were used to expose the investigated teeth in this study: E-speed films (CEA ID, Agfa Healthcare, Mortsel, Belgium) with a spatial resolution of 20 lp/mm, and a photostimulable phosphor plate (PSP) for a direct digital system (Digora



**Fig. 2.** Stereomicroscopic image (32 × magnification) of sectioned tooth shows advanced caries in the proximal surface.

Optime, Soredex, Tuusula, Finland) with a spatial resolution of 12.5 lp/mm and 14-bit grayscale (Fig. 1).

To choose the most appropriate exposure time, different exposure times were tested for each receptor. The shortest exposure times that produced high-quality images, as judged by three examiners, were included in the experiment. Conventional films were processed by an automatic processor (Extra-X, Velopex, London, England).

After being detached from their molds, the teeth were longitudinally separated (mesiodistally) at the middle of their proximal surfaces by using a water-cooled diamond saw. The separated crowns were examined under a stereomicroscope (Leica S 8APO, Microsystem, Heerbrugg, Switzerland) (Fig. 2).

All radiographic images were blindly assessed by three oral radiologists having more than five years of experience

each, with a haphazard arrangement of the images. Each image was assessed twice with a period of two weeks between the two sessions. The radiographic images were evaluated inside a quiet room with dimmed light. A black cardboard with a customized window was placed on a viewer box to be used in the assessment of conventional radiographs, and the use of a magnifying lens ( $2\times$  magnification) was allowed. The digital images were evaluated in such a room by using the Digora for Windows 2.7 software on an 18.5-inch monitor (SyncMaster B1930N, Samsung, Seoul, South Korea) with a resolution of  $1360\times 768$ . The examiners were not allowed to change the contrast and the brightness of the images. Every interpretation session was terminated after 30 min or upon request of any of the examiners because of eye fatigue.

A five-point scoring system was used in the assessment of carious proximal surfaces as follows: 0: sound, 1: incipient caries (less than half the enamel thickness), 2: moderate (more than half the enamel thickness but does not reach the dentino-enamel junction), 3: advanced (less than half the dentin thickness), and 4: severe (more than half the dentin thickness).

The results of radiographic images were compared with those yielded by a stereomicroscope as the gold standard in order to calculate the sensitivity, specificity, positive predictive value (+PV), and negative predictive value (−PV) of both the investigated kVp values in the conventional and the digital images. The receiver operating characteristic (ROC) curve was used to evaluate the diagnostic accuracy measures of the different modalities. Areas under the ROC curve (AUCs) of the different tests were compared

using a  $z$ -statistic. Inter- and intra-observer agreements (reliability) were assessed using the *kappa* statistic. The ROC curve analysis and the reliability analysis were performed with MedCalc Version 11.3 for Windows (MedCalc Software BVBA, Ostend, Belgium).

## Results

Stereomicroscopic findings, the standard reference, revealed that 46.7% of the examined surfaces were carious, while the remaining 53.3% were sound. From the carious surfaces, 31.4% were confined to the enamel (14.3% incipient caries and 17.1% moderate caries) and 68.6% extended into the dentin (25.7% advanced caries and 42.9% severe caries).

With respect to the diagnostic accuracy measures and ROC curve analysis for caries detection using the two imaging modalities and the two kVp settings, conventional radiography (60 kVp) showed the highest sensitivity (74.3%), the highest −PV (77.8%), the highest diagnostic accuracy (77%), and the highest AUC (0.765). Conventional radiography (70 kVp) showed the highest specificity (86.3%) and the highest +PV (80%) (Table 1).

Pair-wise comparisons between the AUC of different caries detection modalities revealed statistically non-significant differences among all modalities.

With respect to the diagnostic accuracy measures and ROC curve analysis for the determination of caries extension into the enamel or the dentin of different modalities, conventional radiography (60 kVp) showed the highest sensitivity (75%). Conventional radiography (70 kVp)

**Table 1.** Results of diagnostic accuracy measures of the four modalities used in the detection of caries

Modality	Sensitivity %	Specificity %	+PV %	−PV %	Diagnostic accuracy %	AUC	SE	95% CI
Conventional (60 kVp)	74.3	78.8	75.4	77.8	77	0.765	0.039	0.689-0.830
Conventional (70 kVp)	62.9	86.3	80	72.6	75	0.746	0.041	0.668-0.813
Digora (60 kVp)	62.9	82.5	75.9	71.7	73	0.727	0.042	0.648-0.796
Digora (70 kVp)	68.6	85	80	75.6	77	0.768	0.039	0.692-0.833

+PV: Positive Predictive Value, −PV: Negative Predictive Value, AUC: Area Under the Curve, SE: Standard Error, CI: Confidence Interval

**Table 2.** Results of diagnostic accuracy measures of the four modalities used in the detection of enamel and dentin caries

Modality	Sensitivity %	Specificity %	+PV %	−PV %	Diagnostic accuracy %	AUC	SE	95% CI
Conventional (60 kVp)	75	86.4	92.3	61.3	81	0.807	0.052	0.695-0.891
Conventional (70 kVp)	70.8	95.5	97.1	60	83	0.831	0.048	0.723-0.910
Digora (60 kVp)	66.7	90.9	94.1	55.6	79	0.788	0.054	0.674-0.877
Digora (70 kVp)	68.8	86.4	91.7	55.9	78	0.776	0.056	0.660-0.867

+PV: Positive Predictive Value, −PV: Negative Predictive Value, AUC: Area Under the Curve, SE: Standard Error, CI: Confidence Interval

**Table 3.** Results of diagnostic accuracy measures of the four modalities used in the detection of incipient and moderate caries

	Modality	Sensitivity %	Specificity %	+PV %	-PV %	Diagnostic accuracy %	AUC	SE	95% CI
Incipient caries	Conventional (60 kVp)	90	63.3	29	97.4	81	0.805	0.062	0.693-0.890
	Conventional (70 kVp)	90	66.7	31	97.6	77	0.772	0.068	0.656-0.864
	Digital (60 kVp)	90	55	25	97.1	74	0.737	0.074	0.619-0.835
	Digital (70 kVp)	90	70	33.3	97.7	78	0.783	0.066	0.669-0.873
Moderate caries	Conventional (60 kVp)	83.3	63.8	32.3	94.9	78	0.779	0.063	0.664-0.869
	Conventional (70 kVp)	91.7	69	37.9	97.6	83	0.831	0.054	0.723-0.910
	Digital (60 kVp)	83.3	72.4	38.5	95.5	81	0.811	0.057	0.700-0.895
	Digital (70 kVp)	75	77.6	40.9	93.7	80	0.801	0.059	0.688-0.887

+PV: Positive Predictive Value, -PV: Negative Predictive Value, AUC: Area Under the Curve, SE: Standard Error, CI: Confidence Interval

**Table 4.** Results of diagnostic accuracy measures of the four modalities used in the detection of advanced and severe caries

	Modality	Sensitivity %	Specificity %	+PV %	-PV %	Diagnostic accuracy %	AUC	SE	95% CI
Advanced caries	Conventional (60 kVp)	100	46.2	39.1	100	68	0.678	0.069	0.555-0.785
	Conventional (70 kVp)	100	44.2	38.3	100	67	0.672	0.069	0.549-0.780
	Digital (60 kVp)	100	48.1	40	100	69	0.688	0.068	0.566-0.793
	Digital (70 kVp)	100	44.2	38.3	100	64	0.639	0.072	0.516-0.751
Severe caries	Conventional (60 kVp)	80	100	100	87	95	0.953	0.028	0.874-0.989
	Conventional (70 kVp)	96.7	85	82.9	97.1	96	0.962	0.025	0.887-0.993
	Digital (60 kVp)	83.3	100	100	88.9	95	0.946	0.030	0.864-0.986
	Digital (70 kVp)	76.7	100	100	85.1	93	0.925	0.036	0.836-0.974

+PV: Positive Predictive Value, -PV: Negative Predictive Value, AUC: Area Under the Curve, SE: Standard Error, CI: Confidence Interval

showed the highest specificity (95.5%), the highest +PV (97.1%), the highest diagnostic accuracy (83%), and the highest AUC (0.831) (Table 2).

Pair-wise comparisons between the AUC of different modalities in the determination of the caries extension into the enamel or the dentin revealed statistically non-significant differences between all modalities.

With respect to the diagnostic accuracy measures and ROC curve analysis for the detection of incipient caries, all modalities showed the same sensitivity (90%). Digital radiography (70 kVp) showed the highest specificity (70%), the highest +PV (33.3%), and the highest -PV (97.7%). Conventional radiography (60 kVp) showed the highest diagnostic accuracy (81%) and the highest AUC (0.805) (Table 3).

With respect to the diagnostic accuracy measures and ROC curve analysis for the detection of moderate caries, conventional radiography (70 kVp) showed the highest sensitivity (91.7%), the highest -PV (97.6%), the highest diagnostic accuracy (83%), and the highest AUC (0.831). Digital radiography (70 kVp) showed the highest specificity (77.6%) and the highest +PV (40.9%) (Table 3).

With respect to the diagnostic accuracy measures and ROC curve analysis for the detection of advanced caries,

all modalities showed a sensitivity of 100%. Digital radiography (60 kVp) showed the highest specificity (48.1%), the highest +PV (40%), the highest diagnostic accuracy (69%), and the highest AUC (0.688). All modalities showed the same -PV (100%) (Table 4).

With respect to the diagnostic accuracy measures and ROC curve analysis for the detection of severe caries, conventional radiography (70 kVp) showed the highest sensitivity (96.7%), the highest -PV (97.1%), the highest diagnostic accuracy (96%), and the highest AUC (0.962). Conventional radiography (60 kVp), digital radiography (60 kVp), and digital radiography (70 kVp) showed the highest specificity (100%) and the highest +PV (100%) (Table 4).

Pair-wise comparisons between the AUC of different modalities in the determination of caries severity revealed statistically non-significant differences among all modalities.

The Kappa statistic showed an inter-observer agreement of 0.754, 0.780, 0.797, and 0.771 for conventional radiography (60 kVp), conventional radiography (70 kVp), digital radiography (60 kVp), and digital radiography (70 kVp), respectively. Further, the intra-observer agreement ranged from 0.765 to 0.790 for conventional radiography (60 kVp),

**Table 5.** Inter-observer and intra-observer agreement results (*Kappa* statistic)

Modality	Inter-observer agreement	Intra-observer agreement (Observer 1)	Intra-observer agreement (Observer 2)	Intra-observer agreement (Observer 3)
Conventional (60 kVp)	0.754	0.790	0.765	0.772
Conventional (70 kVp)	0.780	0.804	0.814	0.790
Digital (60 kVp)	0.797	0.800	0.850	0.803
Digital (70 kVp)	0.771	0.781	0.786	0.774

from 0.790 to 0.814 for conventional radiography (70 kVp), from 0.800 to 0.850 for digital radiography (60 kVp), and from 0.774 to 0.786 for digital radiography (70 kVp) (Table 5).

## Discussion

Upon analyzing the results of the current study, no statistically significant difference in the diagnostic accuracy for the assessment of dental caries in either conventional or digital images could be detected between 60 kVp and 70 kVp. This finding is in contrast to the following statement: “Images with a high contrast are more accurate in caries assessment than those with a low contrast.” This concept, which is stated in textbooks, has been applied in many dental faculties where the oral radiology curricula are based on such textbooks.<sup>24-27</sup> Moreover, some current intraoral X-ray machines allow changing the kilovoltage peak between 60 kVp and 70 kVp, or even between 60 kVp, 65 kVp, and 70 kVp; this option may be partially attributed to the previously mentioned statements about the relationship between short grayscale and caries detection.

When dealing with the assessment of dental caries, sensitivity and specificity as well as positive and negative predictive values have an equivalent diagnostic status. This is because it is important to detect carious lesions in affected teeth as well as to exclude caries in sound teeth. This diagnostic importance is attributed to the fact that false negative cases will lead to the progression of caries, particularly dentine caries, deeper in the tooth with a subsequent more aggressive treatment. Moreover, false positive cases will lead to unrequired restorative intervention. Therefore, it is more practical to deal with the diagnostic accuracy as a whole than dealing with each measure separately.

The results of the current study revealed that the difference between the lower and the higher kilovoltage with respect to the diagnostic accuracy was minor and non-statistically significant. As for conventional radiography, the

use of 60 kVp revealed higher values in the detection of caries and the determination of caries severity in incipient and advanced caries, while the use of 70 kVp showed higher values in the determination of caries extension into the dentin and the determination of caries severity in the cases of moderate and severe caries.

The insignificant importance of changing the kilovoltage values was also evident in digital images but in a different way. The use of 60 kVp showed higher values in the determination of caries extension as well as the severity of moderate, advanced, and severe caries, while the use of 70 kVp aided in caries detection and the determination of its severity in the incipient cases.

These fluctuating results of the high and the low kilovoltage in conventional and digital radiography reflect that changing the tube potential is no longer an influencing factor in caries assessment, the concept that was valid previously on the basis of old studies.<sup>29,30</sup> This finding is not confined to the detection of caries but extends to the determination of caries extension into the enamel and the dentin as well as the severity of the caries.

The non-significant difference between both the investigated kilovoltage peaks in the conventional radiographs may be attributed to the advances in the manufacturing of radiographic films, namely the production of films with a higher film latitude than that of the films produced in the previous decades. In the same manner, the wide dynamic range of digital systems, particularly that of photostimulable phosphor systems, may be the cause for similar results, where a high film latitude and a wide dynamic range permit obtaining diagnostically accepted images with a wide range of exposure time. Based on the fact that the exposure time is the main factor that influences the image density, which will subsequently affect the final contrast of the image, the effect of changing the tube voltage as the master factor determining the image contrast may not be a crucial one.

The results of the current study are consistent with those of Bottenberg et al,<sup>31</sup> who used a charge-coupled device (CCD) and a complementary metal-oxide semiconductor

(CMOS) instead of a PSP, which meant that the non-significant difference in caries assessment between 60 kVp and 70 kVp was not confined only to PSP systems but was also observed in solid-state systems besides conventional radiography.<sup>30,32</sup> The results of previous studies were heterogenous to some extent either because of the use of a non-common kilovoltage<sup>33</sup> or because of the use of the kilovoltage that is not used in intraoral radiography anymore.<sup>34</sup>

Good-to-very good inter-observer and intra-observer agreements for 60 kVp and 70 kVp in both conventional and digital radiography reflected the comparable reliability of both the investigated potentials in the caries assessment. Moreover, the small differences in agreement were not consistent among the study modalities.

In conclusion, the difference between 60 kVp and 70 kVp was not statistically significant with respect to the overall diagnostic accuracy in the dental caries assessment. Moreover, the sensitivity and the specificity as well as the positive predictive value and the negative predictive value in the considered cases were comparable and not constant for either of them in the detection of caries and the determination of its extension into the dentin or its severity. Therefore, from a clinical point of view, changing the tube voltage of intraoral X-ray machines between 60 kVp and 70 kVp has no significant effect on the accuracy of the dental caries assessment, and this lack of effect could exist in both conventional and digital radiography.

## References

- Riley JL 3rd, Gordan VV, Rindal DB, Fellows JL, Ajmo CT, Amundson C, et al. Preferences for caries prevention agents in adult patients: findings from the dental practice-based research network. *Community Dent Oral Epidemiol* 2010; 38: 360-70.
- Kandel EA, Richards JM, Binkley CJ. Childhood caries in the state of Kentucky, USA: a cross-sectional study. *BMC Oral Health* 2012; 12: 38.
- Ayele FA, Taye BW, Ayele TA, Gelaye KA. Predictors of dental caries among children 7-14 years old in Northwest Ethiopia: a community based cross-sectional study. *BMC Oral Health* 2013; 13: 7.
- Colak H, Dülgergil CT, Dalli M, Hamidi MM. Early childhood caries update: a review of causes, diagnoses, and treatments. *J Nat Sci Biol Med* 2013; 4: 29-38.
- Yang J, Dutra V. Utility of radiology, laser fluorescence, and transillumination. *Dent Clin North Am* 2005; 49: 739-52.
- Souza-Zaroni WC, Ciccone JC, Souza-Gabriel AE, Ramos RP, Corona SA, Palma-Dibb RG. Validity and reproducibility of different combinations of methods for occlusal caries detection: an in vitro comparison. *Caries Res* 2006; 40: 194-201.
- Ritter AV, Ramos MD, Astorga F, Shugars DA, Bader JD. Visual-tactile versus radiographic caries detection agreement in caries-active adults. *J Public Health Dent* 2013; 73: 252-60.
- Fuhrmann AW. Current practice in conventional and digital intraoral radiography: problems and solutions. *Int J Comput Dent* 2006; 9: 61-8.
- Wenzel A, Gröndahl HG. Direct digital radiography in the dental office. *Int Dent J* 1995; 45: 27-34.
- Farman AG, Levato CM, Gane D, Scarfe WC. In practice: how going digital will affect the dental office. *J Am Dent Assoc* 2008; 139 Suppl: 14S-9S.
- Vandenbergh B, Jacobs R, Bosmans H. Modern dental imaging: a review of the current technology and clinical applications in dental practice. *Eur Radiol* 2010; 20: 2637-55.
- Haak R, Wicht MJ, Noack MJ. Conventional, digital and contrast-enhanced bitewing radiographs in the decision to restore approximal carious lesions. *Caries Res* 2001; 35: 193-9.
- Price C, Ergül N. A comparison of a film-based and a direct digital dental radiographic system using a proximal caries model. *Dentomaxillofac Radiol* 1997; 26: 45-52.
- Tyndall DA, Ludlow JB, Platin E, Nair M. A comparison of Kodak Ektaspeed Plus film and the Siemens Sidexis digital imaging system for caries detection using receiver operating characteristic analysis. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod* 1998; 85: 113-8.
- Uprichard KK, Potter BJ, Russell CM, Schafer TE, Adair S, Weller RN. Comparison of direct digital and conventional radiography for the detection of proximal surface caries in the mixed dentition. *Pediatr Dent* 2000; 22: 9-15.
- White SC, Yoon DC. Comparative performance of digital and conventional images for detecting proximal surface caries. *Dentomaxillofac Radiol* 1997; 26: 32-8.
- Alkurt MT, Peker I, Bala O, Altunkaynak B. In vitro comparison of four different dental X-ray films and direct digital radiography for proximal caries detection. *Oper Dent* 2007; 32: 504-9.
- Rockenbach MI, Veeck EB, da Costa NP. Detection of proximal caries in conventional and digital radiographs: an in vitro study. *Stomatologija* 2008; 10: 115-20.
- Crombie K, Parker ME, Nortje CJ, Sanderink GC. Comparing the performance of storage phosphor plate and Insight film images for the detection of proximal caries depth. *SADJ* 2009; 64: 452-9.
- Senel B, Kamburoglu K, Uçok O, Yüksel SP, Ozen T, Avsever H. Diagnostic accuracy of different imaging modalities in detection of proximal caries. *Dentomaxillofac Radiol* 2010; 39: 501-11.
- White SC, Pharoah MJ. *Oral radiology: principles and interpretation*. 6th ed. St. Louis: Mosby; 2009.
- Thunthy KH, Manson-Hing LR. Effect of mAs and kVp on resolution and on image contrast. *Oral Surg Oral Med Oral Pathol* 1978; 46: 454-61.
- Helmrot E, Carlsson GA, Eckerdal O, Sandborg M. Influence of scattered radiation and tube potential on radiographic contrast: comparison of two different dental X-ray films. *Dentomaxillofac Radiol* 1991; 20: 135-46.
- Langland OE, Langlais RP, Preece JW. *Principles of dental imaging*. 2nd ed. Baltimore: Lippincott Williams & Wilkins;

- 2002.
25. Johnson ON, McNally MA, Essay CE. Essentials of dental radiography for dental assistants and hygienists. 7th ed. Upper Saddle River: Prentice Hall; 2003.
  26. Iannucci JM, Howerton LJ. Dental radiography: principles and techniques. 3rd ed. St. Louis: Saunders Elsevier; 2006.
  27. Ghom AG. Textbook of oral radiology. Delhi: Elsevier; 2008.
  28. Caldas Mde P, Ramos-Perez FM, de Almeida SM, Haiter-Neto F. Comparative evaluation among different materials to replace soft tissue in oral radiology studies. *J Appl Oral Sci* 2010; 18: 264-7.
  29. Svenson B, Gröndahl HG, Petersson A, Olving A. Accuracy of radiographic caries diagnosis at different kilovoltages and two film speeds. *Swed Dent J* 1985; 9: 37-43.
  30. Svenson B, Petersson A. Influence of tube voltage on radiographic diagnosis of caries in premolars and molars. *Swed Dent J* 1991; 15: 245-50.
  31. Bottenberg P, Jacquet W, Stachniss V, Wellnitz J, Schulte AG. Detection of cavitated or non-cavitated approximal enamel caries lesions using CMOS and CCD digital X-ray sensors and conventional D and F-speed films at different exposure conditions. *Am J Dent* 2011; 24: 74-8.
  32. Svenson B, Welander U, Anneroth G, Söderfeldt B. Exposure parameters and their effects on diagnostic accuracy. *Oral Surg Oral Med Oral Pathol* 1994; 78: 544-50.
  33. Kaepler G, Dietz K, Reinert S. Influence of tube potential setting and dose on the visibility of lesions in intraoral radiography. *Dentomaxillofac Radiol* 2007; 36: 75-9.
  34. Sogur E, Baksı BG, Orhan K, Paksoy SC, Dogan S, Erdal YS, et al. Effect of tube potential and image receptor on the detection of natural proximal caries in primary teeth. *Clin Oral Investig* 2011; 15: 901-7.