



Color variation induced by abutments in the superior anterior maxilla: an *in vitro* study in the pig gingiva

Ramin Atash¹, Mohamed-Reda Boularbah¹, Cetik Sibel^{1,2*}

¹Department of Stomatology and Dentistry, Erasmus Hospital, Université Libre de Bruxelles, Brussels, Belgium

²Laboratory of Physiology and Pharmaceutics, Faculty of Medicine, Université Libre de Bruxelles, Brussels, Belgium

PURPOSE. The aim of this work is to evaluate different types of materials used for making implant abutments, by means of an *in vitro* study and a review of the literature, in order to identify the indications for a better choice of an implant-supported restoration in the anterior section. **MATERIALS AND METHODS.** 5 implant abutments were tested in a random order in the superior anterior maxilla of pig gingiva (n = 8): titanium dioxide (Nobel Biocare); zirconium dioxide, Standard BO shade (Nobel Biocare, Kloten, Switzerland); zirconium dioxide, Light BI shade (Nobel Biocare); zirconium dioxide, Intense A 3.5 shade (Nobel Biocare); and aluminium oxide. Each abutment was tested for 2 mm and 3 mm thickness. To determine color variation, VITA Easyshade Advance spectrophotometer (Vita Zahnfabrik, Bad Sackingen, Germany) was used. **RESULTS.** Results showed that the color variation induced by the abutment would be affected by the abutment material and gingival thickness, when the gingival thickness is 2 mm. All materials except zirconium dioxide (Standard shade) caused a visible change of color. Then, as the thickness of the gingiva increased to 3 mm, the color variation was attenuated in a significant manner and became invisible for all types of abutments, except those made of aluminium oxide. **CONCLUSION.** Zirconium dioxide is the material causing the lowest color variation at 2 mm and at 3 mm, whereas aluminium oxide causes the highest color variation no matter the thickness. [J Adv Prosthodont 2016;8: 423-32]

KEYWORDS. Abutment; Zirconium oxide; Anterior restoration; Gingiva

INTRODUCTION

Nowadays, implantology forms an integral part of dentists' therapeutic arsenal for treating single or multiple missing teeth. Implants are frequently considered to be, and justly so, the optimal solution for reconstructing one or more missing teeth, from both a functional and a psychological

point of view.¹

During the last few years, there has been a remarkable progress in the field of implantology. Initially used solely for denture stabilization, implant dentistry now allows fixed implant-supported dentures for single or multiple missing teeth.² Improvements of surgical methods and the progress in making better osseointegration result in a very high success rate today.²

These particular advances and the technical developments in implantology have created a situation in which the challenges we face are not only adequate osseointegration of the implant, this having already been well mastered, but achieving esthetically better results.

Faced with increasingly demanding patients, practitioners are forced to push back the limits of biomimicry, in order to be able to satisfy them.

After prosthetic restoration of the anterior teeth, the natural appearance of the peri-implant gingiva will be seriously affected by the implant's volume, shape, and color.³

Corresponding author:

Cetik Sibel

Laboratory of Physiology and Pharmaceutics, Faculty of Medicine, Université Libre de Bruxelles, CP 604 808 Route de Lennik, 1070 Brussels, Belgium

Tel. +325556363; e-mail, Sibel.Cetik@ulb.ac.be

Received March 4, 2016 / Last Revision July 22, 2016 / Accepted October 14, 2016

© 2016 The Korean Academy of Prosthodontics

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

Surgical expertise during the actual procedure, good positioning of the implant with regard to the three dimensional space,^{4,5} as well as fine handling of the soft tissues, potentially preceded by increasing the amount of soft tissue,⁶ will be the primary factors for obtaining a harmonious and natural prosthesis-gingiva interface.

The prosthetic phase will play an equally crucial role. During soft tissue healing, the prosthesis will guide the gingiva, in order to obtain a suitable emerging profile. But what about the choice of implant abutment? Histological factors, such as the intensity of melanogenesis, degree of keratinization, and even capillary density, affect color,⁷ and it may also be influenced by the restoration material⁸ and in this particular case by the implant abutment.^{3,9}

The implant abutment will ensure the transition between the implant and the prosthetic tooth. It may be:

- Prefabricated core build-up, modified by reaming intra-orally or in the laboratory
- An individualized abutment, adapted to the gingival margin using a digital procedure (e.g. Procera)
- Castable abutment, but with a machined base for a perfect fit on the implant replicate (e.g. UCLA10 abutment).

Nowadays there are a variety of materials used for making implant abutments,¹⁰ and the four main ones will be included in this study. They may be classified into two categories:

- 1) Metal abutments
 - Titanium
 - Gold
- 2) Ceramic abutments
 - Zirconium dioxide
 - Aluminium oxide

The purpose of this study is to evaluate the different types of materials used for making implant abutments, by means of an *in vitro* study and a review of the literature, in order to identify the indications for a better choice of an implant-supported restoration in the anterior section.

MATERIALS AND METHODS

This study tries to demonstrate the aesthetic properties of materials through an *in vitro* study inspired by Jung *et al.*'s 2007 protocol.³ The study was conducted on 8 different pig maxillae (Fig. 1). These pigs had been slaughtered for food purposes, in accordance with the World Organization for Animal Health standards. Therefore, this study is considered to be an animal study and does not require submission to the FUB-Erasmus Hospital-Faculty Ethics Committee although this committee had been consulted in advance.

Pig gingiva share many similarities with the human keratinized mucosa. In order to be able to simulate different levels of gingival thickness, flaps of 1 mm connective tissue in thickness were removed, from the anterior sector (Fig. 2).

The final thickness of the different sites was measured using an endodontic file (Fig. 3). To minimize artifacts, the different pieces were moistened with saline solution before being superimposed. On each of the sites, 5 implant abutments were tested in a random order:

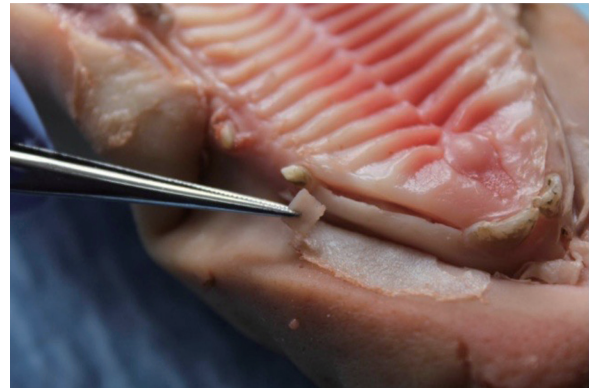


Fig. 1. The site chosen was the anterior part of the superior maxillary area, between the incisors and the canines.



Fig. 2. 1 mm thickness flap, taken at an additional analogous site.

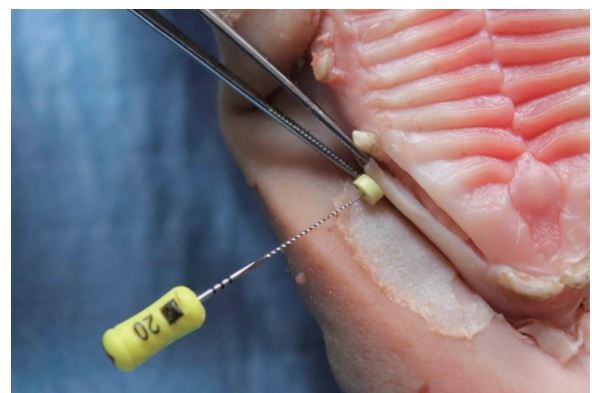


Fig. 3. Measuring gingival thickness using a 20 endodontic file (Dentsply Maillefer, Ballaigues, Switzerland).

- 1) Abutment made of titanium dioxide (Nobel Biocare, Kloten, Switzerland)
- 2) Abutment made of zirconium dioxide, Standard BO shade (Nobel Biocare)
- 3) Abutment made of zirconium dioxide, Light BI shade (Nobel Biocare)
- 4) Abutment made of zirconium dioxide, Intense A 3.5 shade (Nobel Biocare)
- 5) Abutment made of aluminium oxide

In order to objectively evaluate color, a VITA Easyshade Advance spectrophotometer (Vita Zahnfabrik, Bad Sackingen, Germany) was used. Designed for determining tooth color, the device has a VITA SYSTEM 3D- MASTER mode, which also provides the parameters defined by the ICI: L for luminosity, a for absorbance in the red-green range, and b for absorbance in the yellow-blue range.

The site chosen was the superior anterior maxilla. After a full-thickness intrasulcular incision was made with a n° 15 blade, the mucoperiosteal flap was removed using a rugine.

For each operative site, the thickness was measured using an endodontic file, and the first spectrophotometric measurement was recorded by gently placing the spectrophotometer in contact with the gingiva. This site of measurement served as the control site. In each site, we inserted a replica implant (Nobel Biocare) with an internal hexagonal connection.

In a random order, the abutments were placed at the site and the color was analysed using the spectrophotometer. Depending on the thickness measured at the abutment neck, one or more 1 mm-thick flaps were superimposed, in order to simulate a gingival biotype, either thin (2 mm) or thick (3 mm). The 5 abutments were thus tested for each of the two thicknesses (Fig. 4 and Fig. 5). The same manipulation was repeated on the 8 superior maxillae by the same surgeon (Fig. 6). Thus, each abutment (5) was tested twice (2 mm and 3 mm) on 8 pig maxillae.

In order to determine the degree of color variation caused by each abutment, the values of the ICI parameters L, a, and b, measured at the control site were subtracted from those at the test site, and the difference in color (ΔE) produced by each abutment was calculated using the following equation: $\Delta E = (\Delta L^2 + \Delta a^2 + \Delta b^2)^{1/2}$.¹¹ The resulting data was analyzed using the SPSS program, version 22.

The review of the literature for this dissertation was conducted starting with a search on PubMed and the Science Direct Wiley Online Library database, and also using the Google Scholar search engine. The following keywords were used:

‘Abutment’, ‘esthetic abutment’, ‘gingival color abutment’, ‘titanium abutment’, ‘zirconium abutment’, ‘alumina abutment’, ‘gold abutment’, and ‘ceramic abutment’.

For results concerning the aesthetic aspects of abutments, studies done in the years between 2000 and 2014 and, of these, the ones exclusively based on spectrophotometric analysis were chosen, thus excluding the studies of the ‘Pink Aesthetic Score’ type.¹² These studies were clas-



Fig. 4. Placement of the replica implant and positioning of the titanium dioxide abutment (Nobel Biocare, Kloten, Switzerland).

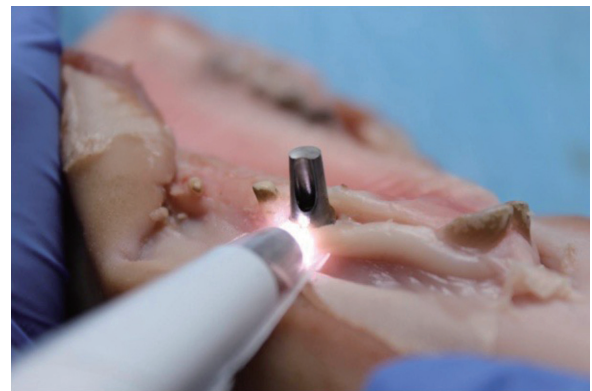


Fig. 5. Recording ICI parameters to determine color variation caused by the abutment, using the VITA Easyshade Advance (Vita Zahnfabrik, Bad Sackingen, Germany).



Fig. 6. Positioning the zirconium dioxide abutment, standard BO shade.

sified and compared using the following parameters: ‘study type’, ‘sample size’, ‘variables studied’, ‘results’, ‘gingival thickness’ and ‘position relative to the marginal limit’ (Table 1).

Table 1. Comparison table of studied parameters and results

| Title | Type of study | Sample Size | Material | Results | Measurement of soft tissue thickness | Vertical distance P/R to marginal limit |
|--|--|--|---|--|--|---|
| Peri-implant soft tissue color around titanium and zirconia abutments: a prospective randomized controlled clinical study | Prospective randomized | 22 | Abutment made of Titanium + CCM vs Abutment made of zirconia + CCC vs Native tooth - Measures before and 1 week after the placement of the crown | - For the two materials \pm significant and visible dE in relation to native tooth - BUT for titanium vs zirconia no significant difference except before placement of the crown, at 1 mm. | YES Measure at 1, 2, and 3 mm. Where the only significant difference has been recorded the thickness was Ti = 1.31 ± 0.69 mm Zi = 1.24 ± 0.35 mm | YES 3 areas of 1 mm. each |
| Spectrophotometric assessment of peri-implant mucosa after restoration with zirconia abutments veneered with fluorescent ceramic: a controlled, retrospective clinical study | Retrospective clinical study | 12 | Zirconia abutment with a fluorescent light orange neck + CCC vs Native tooth | - For zones 1 and 2 In 5/12 difference invisible to the naked eye - whose difference is | NO | 5 areas of 1 mm. each |
| The effect of zirconia and titanium implant abutments on light reflection of the supporting soft tissues | Prospective cross-over type clinical study | 15 | Titanium abutments vs Zirconia Abutments | Significant difference but in relation to gingival thickness : \pm When thickness of the gingiva $> 2 \pm 0.1$ mm, the color difference becomes imperceptible to the naked eye | YES The margin of thickness at which color difference generated by one or the other of the materials is between 0.5 and 2 mm. | YES At 1 mm below the marginal limit Gingival thickness = 2 mm, on average |
| Influence of abutment material on the gingival color of implant-supported all-ceramic restorations: a prospective multicenter study | Prospective study | 20 | - Titanium abutment - Gold abutment - Zirconia abutment vs Native tooth | - The 3 materials \pm color change stat. significant - dE obtained for titanium (11) significantly greater compared to difference observed for Gold (8,9) and Zi (8,5) | YES Division of patients into 2 groups: < 2 mm and > 2 mm \pm No correlation between gingival thickness and color | NO |
| Randomized-controlled clinical trial of customized zirconia and titanium implant abutments for single-tooth implants in canine and posterior regions | Prospective randomized controlled study | 40 implants, 36 been followed-up for 3 years | Zirconia abutment vs Titanium abutment vs Native tooth | - The 2 materials have caused visible color changes - the difference between color changes | YES Gingiva thickness (mean): Zi = 1.9 ± 0.8 mm Ti = 1.7 ± 0.7 mm | NO |

Table 1. (Continued) Comparison table of studied parameters and results

| Title | Type of study | Sample size | Material | Results | Measurement of soft tissue thickness | Vertical distance P/R to marginal limit |
|--|---|-------------|---|---|--|---|
| The effect of all-ceramic and porcelain-fused-to-metal restorations on marginal peri-implant soft tissue color: A randomized controlled clinical trial | Prospective randomized controlled study | 30 | Aluminium oxide abutment + CCC vs Titanium abutment + CCM vs Native tooth | | YES | YES 1 mm below the marginal limit |
| <i>In vitro</i> color changes of soft tissues caused by restorative material | <i>In vitro</i> study | 10 sites | Titanium vs Ti+ceramic vs Zi vs Zi+ceramic | -1.5 mm = All Generating a difference visible to the naked eye -2 mm = Zi and Zi + C does not cause any change visible to the naked eye -3 mm = No change visible for any | YES Thicknesses tested: 1.5 mm 2 mm 3 mm | Study <i>in-vitro</i> , ± not necessary |
| Optical phenomenon of peri-implant soft tissue. Part 1. Spectrophotometric assessment of natural tooth gingiva and peri-implant mucosa | Retrospective clinical study | 15 | Titanium abutments vs Native tooth | Difference of gingival color induced: All results > 3.7 (threshold visible to the naked eye). | NO | YES 5 zones of 1 x 2 mm |
| Optical phenomenon of peri-implant soft tissue. Part II. preferred implant neck color to improve soft tissue aesthetics | Prospective study | 15 | Implant with insertion of colored stripe at the neck vs Native tooth | 8 colors tried, 3 were significantly inferior Light pink : dE 2.12 ± 0.6 Pink = 3.3 ± 0.7 Light orange = 3.4 ± 1 All these results < 3.7 | NO | NO |

RESULTS

Descriptive analyses indicated that for both thicknesses, fitting an implant abutment resulted in a change of color to the peri-implant gingiva (denoted as ΔE), and for all the materials tested (Fig. 7, Table 2).

Subsequently, in order to compare the ΔE values obtained with a human eye threshold under intra-oral conditions, a conformity test with a value of 3.7 was performed, with the null hypothesis being that the material does not cause any visible change of color.

- When gingival thickness was 2 mm, the test rejected

the null hypothesis for all materials tested, with the exception of zirconium dioxide, Standard shade. The result meant that, covered with a 2 mm thickness gingiva, 4 out of 5 of the materials caused visible color changes. These changes were highly significant in the cases of titanium dioxide and aluminium oxide, and they were very highly significant for zirconium dioxide, BI and A3.5 shades (Table 3).

- Moreover, when gingival thickness reached 3 mm, the only visible change was caused by aluminium oxide. This change was highly significant (Table 4).

A t test for paired samples was used to determine the

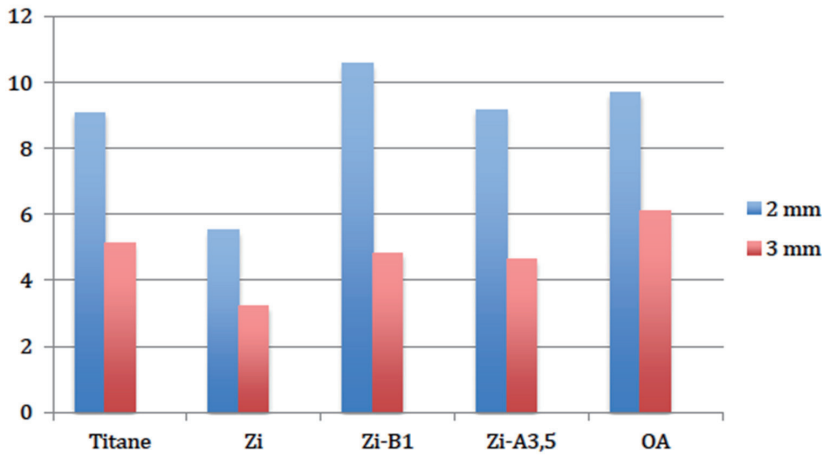


Fig. 7. Diagram of descriptive statistics for the values of LIE color variation, caused by different kinds of abutments, with 2 mm and 3 mm gingival thickness.

Table 2. Descriptive statistics for the values of LIE color variation, caused by different kinds of abutments, with 2 mm and 3 mm gingival thickness

| | N | Minimum | Maximum | Mean | Standard error | Type of difference |
|----------------------------|------------|------------|------------|------------|----------------|--------------------|
| | Statistics | Statistics | Statistics | Statistics | | Statistics |
| Gingival thickness of 2 mm | | | | | | |
| Ti | 8 | 4.0460 | 14.1665 | 9.08313 | 1.481527 | 4.1903 |
| Zi | 8 | 1.5684 | 11.3009 | 5.5057 | 1.19915 | 3.3917 |
| Zi-B1 | 8 | 7.0824 | 15.5255 | 10.5579 | 1.0702 | 3.0270 |
| Zi-A3.5 | 8 | 5.6666 | 10.9129 | 9.1749 | 0.6606 | 1.8684 |
| OA | 8 | 4.4250 | 14.3119 | 9.6840 | 1.1847 | 3.3508 |
| Gingival thickness of 3 mm | | | | | | |
| Ti | 8 | 1.4318 | 5.1127 | 3.3643 | 0.4464 | 1.2627 |
| Zi | 8 | 1.5067 | 6.4645 | 3.2104 | 0.5764 | 1.6303 |
| Zi-B1 | 8 | 2.7185 | 7.7013 | 4.8277 | 0.5817 | 1.6455 |
| Zi-A3.5 | 8 | 2.4940 | 7.0944 | 4.6409 | 0.5941 | 1,6805 |
| OA | 8 | 4.5486 | 8.4581 | 6.1009 | 0.4571 | 1.2928 |

Table 3. 95% conformity test for 3.7 when gingival thickness is 2 mm. Null hypothesis stating that the resulting color variations are equal or inferior to the threshold of 3.7 and that the material does not cause a visible change. The null hypothesis is rejected when Sigma is superior to 0.05

| Single sample test | | | | | | |
|---------------------------|-------|-----------------|------------------|-----------------|--|----------|
| Test value = 3.7 | | | | | | |
| Gingival thickness = 2 mm | | | | | | |
| | t | Deg. of freedom | Sig. (bilateral) | Mean difference | 95% confidence interval for the difference | |
| | | | | | Inferior | Superior |
| Ti | 3.634 | 7 | 0.008 | 5.3833 | 1.8800 | 8.8862 |
| Zi | 1.506 | 7 | 0.176 | 1.8057 | -1.0298 | 4.6413 |
| Zi-B1 | 6.408 | 7 | 0.000 | 6.8579 | 4.3273 | 9.3886 |
| Zi-A3.5 | 8.288 | 7 | 0.000 | 5.4749 | 3.9129 | 7.0369 |
| OA | 5.051 | 7 | 0.001 | 5.9840 | 3.1827 | 8.7853 |

effect of gingival thickness on the color change caused by the abutment. With this test, the results obtained for each abutment at 2 and 3 mm of gingival thickness were compared, with the null hypothesis being that the ΔE color changes caused by each abutment are similar, regardless of the gingival thickness.

The results rejected the null hypothesis for all materials with the exception of zirconium oxide, Standard shade. The difference was significant for aluminium oxide, highly significant for titanium, and very highly significant for zirconium dioxide, BO and A3.5 shades (Table 5).

Table 4. 95% conformity test for 3.7 when gingival thickness is 3 mm. Null hypothesis stating that the resulting color variations are equal or inferior to the threshold of 3.7 and that the material does not cause a visible change. The null hypothesis is rejected when Sigmais superior to 0.05

| Single sample test | | | | | | |
|---------------------------|--------|-----------------|------------------|-----------------|--|----------|
| Test value = 3.7 | | | | | | |
| Gingival thickness = 3 mm | | | | | | |
| | t | Deg. of freedom | Sig. (bilateral) | Mean difference | 95% confidence interval for the difference | |
| | | | | | Inferior | Superior |
| Ti | -0.752 | 7 | 0.477 | -0.3357 | -1.3914 | 0.7200 |
| Zi | -0.849 | 7 | 0.424 | -0.4895 | -1.8525 | 0.8734 |
| Zi-B1 | 1.939 | 7 | 0.094 | 1.1278 | -0.2476 | 2.5031 |
| Zi-A3.5 | 1.584 | 7 | 0.157 | 0.9408 | -0.4641 | 2.3458 |
| OA | 5.253 | 7 | 0.001 | 2.4009 | 1.3201 | 3.4818 |

Table 5. Paired samples test at 95%, null hypothesis stating that for each type of material, the mean values obtained with 2 or 3 mm of gingival thickness are similar. The null hypothesis was rejected for all types of material with the exception of zirconium dioxide, Standard shade.

| Paired samples test | | | | | | | | | |
|---------------------|--|---------|--------------------|----------------------------|--|----------|-------|-------------------|------------------|
| Difference by pair | | | | | | | | | |
| | | Mean | Standard deviation | Standard error of the mean | 95% confidence interval for the difference | | t | Degree of freedom | Sig. (bilateral) |
| | | | | | Inferior | Superior | | | |
| Pair 1 | Ti (2 mm) vs Ti (3 mm) | 5.7188 | 3.2254 | 1.1403 | 3.0223 | 8.4153 | 5.015 | 7 | 0.00154 |
| Pair 2 | Zi (2 mm) vs Zi (3 mm) | 2.2953 | 2.7516 | 0.9728 | -0.0051 | 4.5957 | 2.359 | 7 | 0.05039 |
| Pair 3 | Zi-B1(2 mm) vs Zi-B1 (3 mm) | 5.73026 | 2.3461 | 0.8295 | 3.7688 | 7.6917 | 6.908 | 7 | 0.00023 |
| Pair 4 | Zi-A-3.5 (2 mm) vs Zi-A-3,5 (3 mm) | 4.5341 | 2.3384 | 0.8268 | 2.5791 | 6.4890 | 5.484 | 7 | 0.00092 |
| Pair 5 | QA (2 mm) vs QA (3 mm) | 3.5831 | 3.7983 | 1.3429 | 0.4076 | 6.7588 | 2.668 | 7 | 0.03208 |

DISCUSSION

Our *in vitro* study proves that implant abutment placement causes color change to the overlying gingiva, the change having little to do with the type of material from which the abutment is made. This color change, which can be unsightly and compromise the aesthetic success of implant prosthetic treatment, is variable depending on type of material and gingival thickness.

In our study, when gingival thickness was 2 mm, only an abutment made of zirconium dioxide, Standard shade, did not result in a visible change of color. When we simulated a 3 mm thickness gingival biotype, all of the color changes were reduced, except in the case of zirconium, which already had a value below the visibility threshold. Finally, only aluminium oxide resulted in a visible color change each time.

The small sample size and the *in vitro* nature of the study imply that these results should be interpreted with caution. In the scientific literature, many cases of a greyish peri-implant discolouration of the gingiva have been previously reported (Table 1).¹³ After many case report publications, these discolourations were objectively measured *in vivo*, for the first time, by Jung *et al.*⁹ in 2008, using spectrophotometric measurements in a randomized, prospective, clinical study. They showed that the placement of a titanium abutment caused visible gingival discolouration that was unsightly and inharmonious with the adjacent tooth's gingiva.

Numerous materials are used to make implant abutments, and these can be classified into two main categories:

Metal abutments can be made of titanium or gold. These abutments were the first to be used. Titanium is a rigid material that breaks when submitted to forces. Titanium abutments have ease of use and they have excellent biocompatibility features¹⁴ combined with a minimal risk of corrosion when coming into contact with the implant.¹⁵ This is also the material where most clinical experience has been gained.

The majority of abutments made of a gold alloy are UCLA type abutments. Gold is a material that suffers from distortion when submitted to forces. These abutments are made up of a machined golden part, combined with a plastic sheath cast onto an alloy of precious metals (a gold-palladium alloy).¹⁰ This method will allow abutments to be made so they are adapted to the clinical situation, in relation to both gingival contour and angulation. However, according to the study by Andersson *et al.*,¹⁶ even though gingival discolourations around golden abutments appeared to be significantly lower than discolourations around a titanium abutment, they still remained visible, when compared to the natural tooth.

For Jung *et al.*,⁹ this type of abutment also caused a peri-implant gingival discolouration that was significant and visible.

In order to reduce unsightly gingival discolouration, various kinds of ceramic abutments have been designed: aluminium oxide and zirconium oxide abutments.

Presented in a prospective, randomized clinical study by Jung *et al.*,⁹ abutments made of aluminium oxide exhibited excellent optical properties, causing significantly weaker

variation of gingival color, compared to titanium or golden abutments. They were made up of more than 99.5% aluminium oxide with traces of magnesium oxide, calcium and alkali metals. Unfortunately, with a flexion resistance of only 520 MPa, abutments made of aluminium oxide have shown the limits of their mechanical properties and numerous cases of fracture have been recorded.¹⁶

Zirconium oxide abutments are made from tetragonal polycrystalline zirconium, stabilized with yttrium oxide, is, due to its excellent mechanical properties being both resistant and of fine texture, the ceramic is the material of choice, especially for frame design in fixed prosthesis.¹⁷ *In vitro*, its mechanical resistance is twice that of aluminium oxide, with a flexion resistance of 1120 MPa.¹⁸ In an *in vivo* study, Rimondini *et al.*¹⁹ have shown that bacterial adhesion to zirconium oxide abutments was significantly lower than that to titanium oxide abutments.

Regarding optical properties, the studies were not entirely in agreement, but the authors^{3,9,20,21} agreed on the fact that zirconium oxide abutments caused a color change to the peri-implant gingiva. This change was significantly lower than the change caused by either titanium or gold, but it remained visible in the *in vivo* studies.

Subsequently, laboratories offered a multitude of shades for zirconia abutments, incorporating pigmented powders during the material's preparation, as was the case for the zirconia light BI shade and intense A 3.5 shade abutments used in our study.

Even though there were, indeed, multiple studies regarding discolouration caused by implant abutments, the results did not always overlap. However, these differences might be explained, in part, by multiple factors that are the evaluation of gingival color, the differences at the tested sites, grafted sites, the measurement of soft tissue thickness, the method for measuring gingival thickness and the Correlation between gingival thickness and optimal choice of abutment.

In order to evaluate the color of each site in an objective and replicable manner, the values of the following parameters were recorded: Luminosity (L), absorbance in the red-green range (a) and absorbance in the yellow-blue range (b). These values were either directly recorded at the site using a spectrophotometer, or they were collected after digital analysis of site pictures. Therefore, there was already a first difference in the method of data acquisition for color-related data. This data has allowed us to study color variation between different sites, in accordance with the recommendations of the International Commission on Luminosity (1976): $\Delta E = (\Delta L^2 + \Delta a^2 + \Delta b^2)^{1/2}$.

Meanwhile, in order for it to be pertinent, the ΔE value must be compared to the threshold perceived by the human eye.

Under laboratory conditions,²² the human eye can distinguish a color variation equal to $\Delta E = 1$. However, inside the oral cavity, this capability decreases and the variation has to be $\Delta E > 3.7$ to be clinically discernible.²³

In order to study color variation caused by the abutment, compared to a control site, only two studies.^{20,21} have

followed a cross-over protocol, alternating different abutments on the same test site in a random order. In this event, the protocol may bring the risk that the results might be biased, either due to pre-existing heterogeneity of the gingival color²⁴ between two adjacent sites, heterogeneity that may reach a value of $\Delta E = 2.7$, or gingival color differences between two groups of patients to be excluded.¹³

Certain studies^{9,25} included a group of patients who had benefited from a connective tissue autograft on the test site. It cannot be neglected that this tissue augmentation may cause residual variation to the gingival color.

Not all studies on gingival peri-implant discolouration measure gingival thickness. It does, however, seem legitimate to think that a particular thickness might affect (or not) the diffusion of discolouration caused by implant abutments (cf. 6).

Out of 10 studies comparing different materials using a spectrophotometer, only 7 included gingival thickness as a parameter. In our study, gingival thickness has played a significant role and, when it was 3 mm, the changes caused by titanium and zirconia abutments fell under the visibility threshold.

The thickness was measured either directly at the site level using an endodontic file, or indirectly, on a digital photograph or on the laboratory replica model. A measurement bias may therefore be present and, at this point, there is no published study comparing the efficacy of these methods for measuring soft tissue thickness.

In an *in vitro* study,³ comparing Ti and Zi with and without fixed ceramic material, all of the materials caused visible ΔE when the gingival thickness was equal to 1.5 mm. At 2 mm, only Ti caused a visible ΔE . Finally, when the gingival thickness was ≥ 3 mm, no material caused a visible ΔE . This study clearly establishes an association between gingival thickness and the indication of the material of choice, in relation to the gingival thickness.

A prospective randomized study by this same group of researchers,⁹ comparing aluminium oxide abutments with titanium ones, showed an ΔE that was significantly lower for the aluminium oxide. However, the group with an aluminium oxide abutment had a mean gingival thickness of 3.4 ± 1.4 mm, against a thickness of 2.9 ± 0.9 mm in the titanium abutment group. This mean difference of 0.5 mm might, at least in part, explain the difference between those two thicknesses.

In a prospective study, Andersson *et al.*¹⁶ divided patients in two groups (≤ 2 mm and > 2 mm of thickness) and concluded that there was no association between gingival thickness and induced color change and that titanium, zirconia, and gold resulted in a visible ΔE even though the values were significantly less significant for gold and zirconia, compared to titanium. Nevertheless, it should be clarified that the patients in the sample had a quite thin gingiva as there was no patient with a gingival thickness of ≥ 3 mm.

In the study by Zembic *et al.*,²⁵ both zirconia and titanium caused visible ΔE , similar in value. In this study, gingival thickness was approximately 1.9 ± 0.8 in the zirconia arm

and 1.7 ± 0.4 mm in the titanium arm. van Brakel *et al.*²¹ came to the conclusion that no visible ΔE was acquired from a thickness equal or greater than 2 ± 0.1 mm, either in titanium or zirconia. Cosgarea *et al.*¹³ stated that when mean gingival thickness ranged from 1.02 ± 0.36 mm to 2.27 ± 0.34 mm, titanium and zirconia abutments both resulted in significant final visible ΔE s, with no association with gingival thickness having been noted. One must also note the small mean gingival thickness of this particular sample and the absence of a graft case.

Evidently, there is lack of standardization among the studies and the different results do not allow the establishment of an exact limit of gingival thickness, beyond which no type of material results in visible discolouration. The only study clearly establishing an association between gingival thickness and the material used, an association characterized by ΔE inferior to the visible threshold, was an *in vitro* study.¹³ However, all *in vivo* studies seemed to converge towards the fact that, as long as the mean gingival thickness of the sample was ≤ 2 mm, the implant abutment caused a visible change to the gingival color, no matter what the material was. Zirconia and aluminium oxide caused a color variation that was less pronounced but still remained visible. In our results, only Standard shade zirconia caused a non visible color change in thin gingiva.

For the majority of clinical studies, abutments made of zirconia (thought to be more aesthetic) seem to cause gingival discolouration to a lesser degree than titanium abutments. This discolouration remains visible in certain cases. Other strategies are being studied, aiming to improve the aesthetics of implant-supported restorations of the anterior sector.

In a retrospective clinical study, Happe *et al.*²⁶ proposed individualised zirconia abutments, modified with a 2 mm ceramic neck, of clear orange fluorescent color to 12 patients needing an implant in the anterior sector. The results, obtained with spectrophotometric analysis, were promising; the color variation induced in 5 of the 12 patients was below the threshold and was visible to the naked eye. However, it must be made clear that this particular study excluded patients with a gingival thickness of ≤ 2 mm. The gingival biotype was quite thick, a factor that could partially explain the results. Ishikawa-Nagai *et al.*²⁷ equally obtained the results below the threshold distinguishable to the naked eye, proposing the implants with a neck of light pink or light orange color. The idea of using the most natural colors in order to mimic the natural gingiva seems equally interesting.

CONCLUSION

With reservations inherent to the limits of an *in vitro* study, we could state that all implant abutments caused a colour change to the overlying gingiva. However, we may also conclude that zirconium dioxide, Standard shade, is the material causing the lowest colour variation. Therefore, zirconium dioxide makes the most appropriate choice for limiting gin-

gival colour variation.

ORCID

Mohamed-Reda Boularbah <http://orcid.org/0000-0002-0446-5660>

Cetik Sibel <http://orcid.org/0000-0001-8338-3921>

REFERENCES

- Torabinejad M, Anderson P, Bader J, Brown LJ, Chen LH, Goodacre CJ, Kattadiyil MT, Kutsenko D, Lozada J, Patel R, Petersen F, Puterman I, White SN. Outcomes of root canal treatment and restoration, implant-supported single crowns, fixed partial dentures, and extraction without replacement: a systematic review. *J Prosthet Dent* 2007;98:285-311.
- Baudouin CA, Bennani V. Esthétique et profil d'émergence en implantologie. 1st ed. Paris: Cahiers de Prothese; 2000.
- Jung RE, Sailer I, Hämmerle CH, Attin T, Schmidlin P. In vitro color changes of soft tissues caused by restorative materials. *Int J Periodontics Restorative Dent* 2007;27:251-7.
- Tarnow DP, Wagner AW, Fletcher P. The effect of the distance from the contact point to the crest of bone on the presence or absence of the interproximal dental papilla. *J Periodontol* 1992;63:995-6.
- Tarnow D, Elian N, Fletcher P, Froum S, Wagner A, Cho SC, Salama M, Salama H, Garber DA. Vertical distance from the crest of bone to the height of the interproximal papilla between adjacent implants. *J Periodontol* 2003;74:1785-8.
- Soadoun AP, Touati B. Soft tissue recession around implants: Is it still unavoidable?-Part II. *Pract Proced Aesthet Dent* 2007;19:81-7.
- Kleinheinz J, Büchter A, Fillies T, Joos U. Vascular basis of mucosal color. *Head Face Med* 2005;1:4.
- Takeda T, Ishigami K, Shimada A, Ohki K. A study of discoloration of the gingiva by artificial crowns. *Int J Prosthodont* 1996;9:197-202.
- Jung RE, Holderegger C, Sailer I, Khraisat A, Suter A, Hämmerle CH. The effect of all-ceramic and porcelain-fused-to-metal restorations on marginal peri-implant soft tissue color: a randomized controlled clinical trial. *Int J Periodontics Restorative Dent* 2008;28:357-65.
- Davarpanah M, Szmukler-Moncler S, Rajzbaum P, Davarpanah K, Demurashvili G. Manuel d'implantologie clinique. 3rd ed. Paris, Cahier de Prothese; 2013. p. 309-12.
- Fürhauser R, Florescu D, Benesch T, Haas R, Mailath G, Watzek G. Evaluation of soft tissue around single-tooth implant crowns: the pink esthetic score. *Clin Oral Implants Res* 2005;16:639-44.
- Johnston WM, Kao EC. Assessment of appearance match by visual observation and clinical colorimetry. *J Dent Res* 1989; 68:819-22.
- Cosgarea R, Gasparik C, Ducea D, Culic B, Dannewitz B, Sculean A. Peri-implant soft tissue colour around titanium and zirconia abutments: a prospective randomized controlled clinical study. *Clin Oral Implants Res* 2015;26:537-44.
- Picard B. Biomateriaux métalliques et biocompatibilité. Implantologie. Paris, Masson, 1992.
- Bert M, Missika P. Les clés du succès en implantologie, 1st ed. Paris, Cahiers de Prothese; 2009.
- Andersson B, Taylor A, Lang BR, Scheller H, Schärer P, Sorensen JA, Tarnow D. Alumina ceramic implant abutments used for single-tooth replacement: a prospective 1- to 3-year multicenter study. *Int J Prosthodont* 2001;14:432-8.
- Raigrodski AJ. Contemporary materials and technologies for all-ceramic fixed partial dentures: a review of the literature. *J Prosthet Dent* 2004;92:557-62.
- Yildirim M, Fischer H, Marx R, Edelhoff D. In vivo fracture resistance of implant-supported all-ceramic restorations. *J Prosthet Dent* 2003;90:325-31.
- Rimondini L, Cerroni L, Carrassi A, Torricelli P. Bacterial colonization of zirconia ceramic surfaces: an in vitro and in vivo study. *Int J Oral Maxillofac Implants* 2002;17:793-8.
- Bressan E, Paniz G, Lops D, Corazza B, Romeo E, Favero G. Influence of abutment material on the gingival color of implant-supported all-ceramic restorations: a prospective multicenter study. *Clin Oral Implants Res* 2011;22:631-7.
- van Brakel R, Noordmans HJ, Frenken J, de Roode R, de Wit GC, Cune MS. The effect of zirconia and titanium implant abutments on light reflection of the supporting soft tissues. *Clin Oral Implants Res* 2011;22:1172-8.
- Johnston WM, Kao EC. Assessment of appearance match by visual observation and clinical colorimetry. *J Dent Res* 1989; 68:819-22.
- Kuehni RG, Marcus RT. An experiment in visual scaling of small color differences. *Colour Res Application* 1979;4:83-91.
- Ishikawa S, Nemoto F, Furukawa K, Ishibashi K. Colorimetric studies of the gingiva. Color variation of the gingiva in the upper anterior region. *Nihon Hotetsu Shika Gakkai Zasshi* 1988;32:821-8.
- Zembic A, Sailer I, Jung RE, Hämmerle CH. Randomized-controlled clinical trial of customized zirconia and titanium implant abutments for single-tooth implants in canine and posterior regions: 3-year results. *Clin Oral Implants Res* 2009; 20:802-8.
- Happe A, Schulte-Mattler V, Fickl S, Naumann M, Zöller JE, Rothamel D. Spectrophotometric assessment of peri-implant mucosa after restoration with zirconia abutments veneered with fluorescent ceramic: a controlled, retrospective clinical study. *Clin Oral Implants Res* 2013;24:28-33.
- Ishikawa-Nagai S, Da Silva JD, Weber HP, Park SE. Optical phenomenon of peri-implant soft tissue. Part II. Preferred implant neck color to improve soft tissue esthetics. *Clin Oral Implants Res* 2007;18:575-80.