



# Dosimetric Analysis on the Effect of Target Motion in the Delivery of Conventional IMRT, RapidArc and Tomotherapy

Ju-Young Song

Department of Radiation Oncology, Chonnam National University Medical School, Gwangju, Korea

**Received** 13 November 2017

**Revised** 11 December 2017

**Accepted** 11 December 2017

**Corresponding author**

Ju-Young Song

([jysong@jnu.ac.kr](mailto:jysong@jnu.ac.kr))

Tel: 82-61-379-7225

Fax: 82-61-379-7249

One of the methods to consider the effect of respiratory motion of a tumor target in radiotherapy is to establish a treatment plan with the internal target volume (ITV) created based on an accurate analysis of the target motion displacement. When this method is applied to intensity modulated radiotherapy (IMRT), it is expected to yield a different treatment dose distribution under the motion condition according to the IMRT method. In this study, we prepared ITV-based IMRT plans with conventional IMRT using fixed gantry angle beams, RapidArc using volumetric modulated arc therapy, and tomotherapy using helical therapy. Then, the variation in dose distribution caused by the target motion was analyzed by the dose measurement in the actual motion condition. A delivery quality assurance plan was prepared for the established IMRT plan and the dose distribution in the actual motion condition was measured and analyzed using a two-dimensional diode detector placed on a moving phantom capable of simulating breathing movements. The dose measurement was performed considering only a uniform target shape and motion in the superior-inferior (SI) direction. In this condition, it was confirmed that the error of the dose distribution due to the target motion is minimum in tomotherapy. This is thought to be due to the characteristic of tomotherapy that treats the target sequentially by dividing it into several slices. When the target shape is uniform and the main target motion direction is SI, it is considered that tomotherapy for the ITV-based IMRT method has a characteristic which can reduce the dose difference compared with the plan dose under the target motion condition.

**Keywords:** Internal target volume (ITV), RapidArc, Tomotherapy, Tumor motion, MapCHECK2

## Introduction


Many methods have been researched and developed to reduce the effect of respiratory motion of tumor targets during radiotherapy. These can be categorized into two main methods in the clinical practice. One is the gating and active breathing control (ABC) method, which allows irradiation only of a stable part of the tumor motion range.<sup>1-4)</sup> The other is to construct a treatment field based

on the internal target volume (ITV) setting using four-dimensional computed tomography to accurately cover the whole area of the motion of the tumor target.<sup>5,6)</sup> A gating method can theoretically be considered as the optimal method to minimize the side effects on the surrounding normal tissue, because it can reduce the size of the treatment field. However, it has a limitation that it requires regular and stable respiration of the treated patients and it cannot be applied to all treatment machines. Therefore, it

is more commonly used to set the treatment field based on the accurate ITV setting that can be applied to all treatment devices.

In the case of ITV-based radiotherapy, the dose distribution of the general 3-dimensional conformal radiotherapy (3D CRT) is considered to be the same as the calculated dose distribution in the treatment area. However, when the dose distribution changes dynamically according to the motion of the multi-leaf collimator (MLC) as in the intensity-modulated radiotherapy (IMRT), the change in the actual dose distribution due to tumor movement is expected to be significant.<sup>7-11)</sup>

The purpose of this study was to analyze the dose variation in the ITV-based IMRT treatment due to the respiratory motion, compared with the calculated dose distribution in the plan according to the IMRT performance technique. The ITV for the virtual tumor target for the phantom was set and the organ at risk volume (OAR) was delineated around it; three different IMRT plans, a fixed-gantry IMRT, a volumetric modulated arc therapy (VMAT), and tomotherapy (Accuray, Sunnyvale, CA, USA) using helical therapy were prepared separately. Delivery quality assurance (DQA) plans were established for these treatment plans, and dose distributions were measured under actual motion conditions. The dose variations were compared and analyzed for each treatment method in order to evaluate the effect of a target motion on the IMRT dosimetric error.

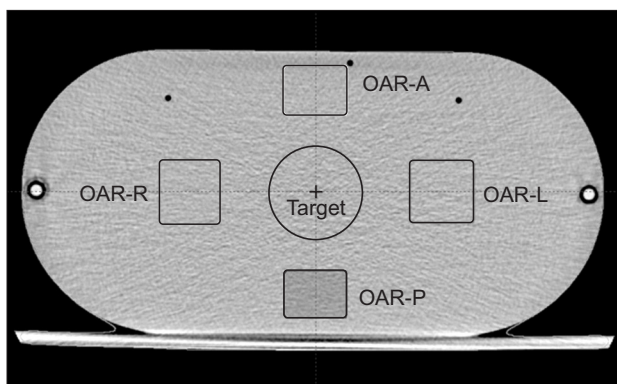

**Fig. 1.** Virtual tumor target and peripheral organs at risk for the preparation of IMRT plan.

## Materials and Methods

### 1. IMRT plan preparation

IMRT Phantom (IBA, Schwarzenbruck, Germany) CT images were acquired and IMRT treatment plans were prepared by creating a virtual tumor target and peripheral OARs, as shown in Fig. 1.

The shapes of the tumors were cylindrical, with a diameter of 6 cm and lengths of 2, 4, and 6 cm. The surrounding major organs were placed on a square column of side length 4 cm with height equal to that of the tumor and placed 3 cm away from the tumor in the up-down direction and 2 cm in the left-right direction.

The tumor movement related to the ITV setting was considered only in the superior-inferior (SI) direction, owing to the limited direction of movement of the moving phantom, and the motion condition was applied to two motion ranges of 4 cm and 2 cm and two motion periods of 7 s and 4 s. Table 1 shows the five ITV setting conditions used in this study.

The IMRT treatment plan was based on the Novalis TX (Varian, PaloAlto, CA, USA) linear accelerator. A RapidArc (Varian, PaloAlto, CA, USA) plan with one arc and an IMRT plan consisting of seven fixed gantry angular beams (FB-IMRT) was established using the Eclipse (Varian, PaloAlto, CA, USA) treatment planning system (TPS). A tomotherapy plan was established in addition and a total of three

**Table 1.** The length of internal target volume (ITV) according to the motion range of clinical target volume (CTV) considered in this study.

CTV length	Motion range	
	2 cm	4 cm
2 cm	4 cm	6 cm
4 cm	6 cm	8 cm
6 cm	8 cm	

**Table 2.** Dose constraints in the optimization process of the IMRT planning.

ITV	$V_{4,750 \text{ cGy}} > 98\%$
OAR_L	$D_{\max} < 2,500 \text{ cGy}$ , $D_{\text{mean}} < 1,200 \text{ cGy}$
OAR_R	$D_{\max} < 2,800 \text{ cGy}$ , $D_{\text{mean}} < 1,000 \text{ cGy}$
OAR_S	$D_{\max} < 2,500 \text{ cGy}$
OAR_I	$D_{\max} < 2,000 \text{ cGy}$

separate IMRT treatment techniques were prepared. The total prescription dose was 5,000 cGy for the ITV in 25 fractions and was optimized according to the constraints in Table 2. All the plans were made to meet the constraint conditions.

## 2. Measurement of IMRT dose distribution under the motion condition

A DQA plan for each treatment plan was created and applied to the dose measurement in order to analyze the changes in dose distribution during beam irradiation of each of the three IMRT methods under the motion conditions. The DQA plan was based on a CT image of MapCHECK2 (SunNuclear, Melbourne, FL, USA), a 2D diode detector array, inserted into MapPHAN (SunNuclear, Melbourne, FL, USA), a solid water phantom, and a Dynamic Platform Model 008PL (CIRS, Norfolk, VA, USA) moving phantom was used to simulate the motion conditions. Phantom setup images for the dose measurements using the NovalisTx and tomotherapy instruments are shown in Fig. 2 and Fig. 3.

The dose measurements were performed for various combinations of motion ranges, 2 cm and 4 cm, and motion periods, 7 s and 4 s. The errors from the dose distribution in the original plan were compared and analyzed by gamma evaluation with a 3% dose difference and 3-mm distance-to-agreement criterion.



**Fig. 2.** Phantom setup image for the dose measurement in the Novalis Tx.

## Results

The dose distribution measured with MapCHECK2 under various motion conditions was slightly different for each treatment method, and Fig. 4 shows an example of these different results.

The calculated pass rates by the gamma evaluation for each clinical target volume (CTV) tumor size in the condition of motion are shown in Tables 3, 4, and 5.

As shown in the pass rates of the tables, the average difference in pass rate between the 4 s and 7 s period was  $0.18 \pm 0.73\%$  in the case of tomotherapy,  $1.44 \pm 2.16\%$  in the case of RapidArc, and  $-0.52 \pm 0.97\%$  in the case of FB-IMRT. For RapidArc, the pass rate difference at 4 s was slightly higher than those for tomotherapy and FB-IMRT, but the mean of the overall difference was  $0.29 \pm 1.73\%$ , indicating that the change in motion period had little effect on dose accuracy.

The factors that have the greatest influence on the dose distribution in the motion condition are the magnitude of motion range, which can be confirmed in the table results. It was confirmed that the dose error was further increased with increasing motion range because the pass rate was lower at the 4-cm motion range than at the 2-cm motion range.

The degree to which the error increased with increasing motion range showed different tendencies according to the treatment method. In the case of tomotherapy, the mean pass rate was  $83.08 \pm 0.78\%$  at the 4-cm motion range and  $95.80 \pm 0.72\%$  at the 2-cm motion range. In the



**Fig. 3.** Phantom setup image for the dose measurement in the Tomotherapy.

case of RapidArc, the mean pass rate was  $63.68 \pm 5.08\%$  at the 4-cm motion range and  $81.43 \pm 3.81\%$  at the 2-cm motion range. For FB-IMRT, the average pass rate was  $61.38 \pm 6.49\%$  for 4 cm motion range and  $82.05 \pm 4.67\%$  for 2 cm motion range. As shown by the above results, the

tendency of the dose error increase with the increase in the motion displacement from 2 cm to 4 cm was different according to the treatment technique. The mean decrease in pass rate was  $-12.50 \pm 1.19\%$  in the case of tomotherapy,  $-18.88 \pm 8.27\%$  in the case of RapidArc, and  $-21.95 \pm 8.96\%$  in

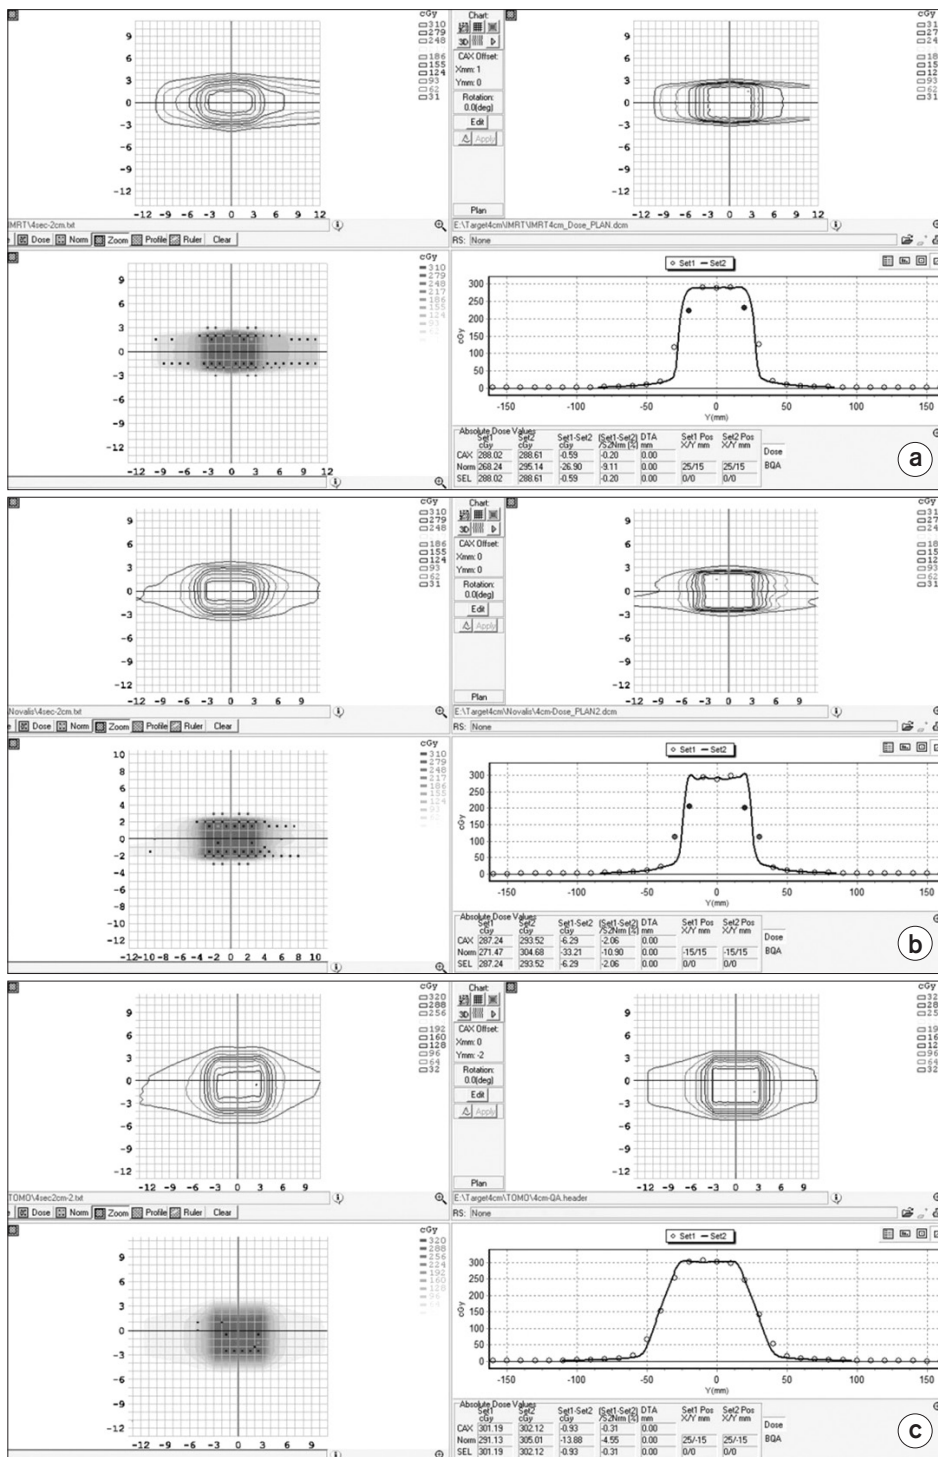


Fig. 4. Example of the measured dose distribution and error analysis in the moving condition. (a) RapidArc, (b) FB-IMRT, (c) Tomotherapy.

**Table 3.** The calculated pass rates by the gamma evaluation for the CTV with 2 cm length in the condition of motion.


	ITV length	Static condition	7 sec motion period		4 sec motion period	
			4 cm range	2 cm range	4 cm range	2 cm range
RapidArc	4 cm	100.0%		77.7%		76.0%
	6 cm	99.7%	59.0%		60.2%	
FB-IMRT	4 cm	100.0%		76.7%		77.1%
	6 cm	100.0%	55.9%		55.6%	
Tomotherapy	4 cm	100.0%		96.3%		96.6%
	6 cm	100.0%	83.0%		82.0%	

**Table 4.** The calculated pass rates by the gamma evaluation for the CTV with 4 cm length in the condition of motion.

	ITV length	Static condition	7 sec motion period		4 sec motion period	
			4 cm range	2 cm range	4 cm range	2 cm range
RapidArc	6 cm	99.7%		83.3%		82.4%
	8 cm	99.5%	65.5%		70.0%	
FB-IMRT	6 cm	100.0%		82.2%		81.9%
	8 cm	100.0%	67.0%		67.0%	
Tomotherapy	6 cm	100.0%		95.7%		95.9%
	8 cm	100.0%	83.6%		83.7%	

**Table 5.** The calculated pass rates by the gamma evaluation for the CTV with 6 cm length in the condition of motion.

	ITV length	Static condition	7 sec motion period	4 sec motion period
			2 cm range	2 cm range
RapidArc	8 cm	99.5%	83.1%	86.1%
FB-IMRT	8 cm	100.0%	88.4%	86.0%
Tomotherapy	8 cm	100.0%	94.5%	95.8%

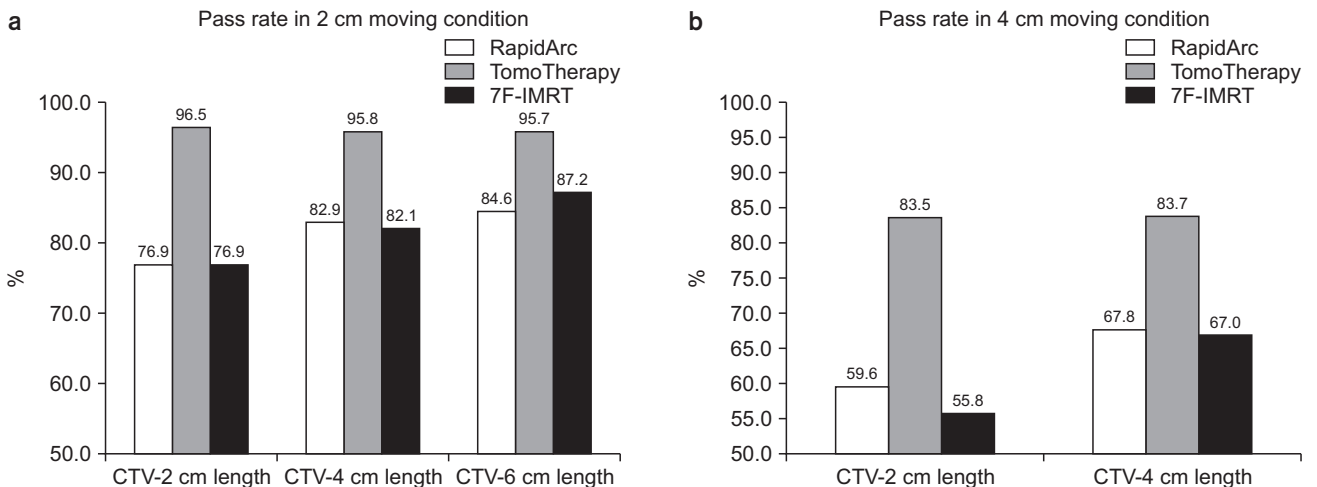

**Fig. 5.** Graphs showing the effect of target motion according to the CTV increase due to CTV length increase. (a) Pass rate in 2 cm moving condition. (b) Pass rate in 4 cm moving condition.

the case of FB-IMRT. These results show that the dose error due to the increase in the motion range was relatively small in tomotherapy compared to those in RapidArc and FB-

IMRT.

The effect of target motion according to the CTV increase due to CTV length increase is shown in Fig. 5. In the case



of the 2-cm motion range, the dosimetric error according to the decrease in CTV increased by 0.8% in tomotherapy, 7.7% in RapidArc, and 10.3% in FB-IMRT. In the case of 4-cm motion range, the dosimetric error according to the decrease in CTV increased by 0.2% in tomotherapy, 8.2% in RapidArc and 11.2% in FB-IMRT. Although there was no significant difference in tomotherapy, the pass rate was lower and the dosimetric error was relatively increased in the case of RapidArc and FB-IMRT, as the CTV was smaller due to the shorter CTV length.

## Discussion

We analyzed how the target motion affects the changes in dose distribution in the ITV-based IMRT according to the IMRT method.

As can be seen from the results, the influence of the tumor motion period on the difference in the dosimetric error was not significant, and the magnitude of the motion range of the tumor was the most influential factor for the dosimetric error. The most important aspect of controlling the effect of tumor movement is the magnitude of the displacement of the movement. It is important to reduce the ITV area by maintaining a shallow breathing pattern rather than a regular breathing pattern. It is considered that this method can reduce the error of an ITV-based IMRT dose distribution.

Because the shape of the target used in the analysis was relatively uniform and the motion direction was considered only in the SI direction, the change in dose due to motion mainly occurred at the tip of the target. However, the pattern showed slightly different dose changes according to the characteristics of the tomotherapy, RapidArc and FB-IMRT treatment methods. Since FB-IMRT and RapidArc deliver the treatment beam for the entire target, the point where the dose distribution error by gamma evaluation exceeds the reference value is more widely spatially distributed. Owing to the characteristics of the helical treatment method, tomotherapy was mainly distributed to the dose error point in the target moving SI direction, and the dose error at the end positions of the target was dominant. This was thought to be the cause of the smallest change in dose with tumor motion in tomotherapy among

the three types of IMRT treatment. The target motion in a relatively uniform shape is considered to cause a relatively low dose distribution error due to motion in tomotherapy, compared to the case where the IMRT dose is irradiated to the entire target in the treatment process. This is due to the characteristic of the helical therapy, which treats multiple sectors of the target sequentially. Although it may be a little different when the target shape is complex and the direction of motion is three-dimensionally complex, as a result of the sequential treatment characteristics of tomotherapy, it is expected that there will be a lower dose error than for other IMRT methods. Based on these results, tomotherapy is considered to be more proper to keep the similar dose compared with the original plan of ITV-based IMRT than other IMRT methods when the gating method cannot be applied to reduce target motion effects.

Although many studies have been carried out on the motional effects of target and OARs on the treatment of tomotherapy, a clinically applicable method that can reduce the motional effect like a gating method has not been developed yet.<sup>12-14)</sup> Therefore, it is inevitable to establish a treatment plan based on ITV and to perform treatment in tomotherapy. In the case of patients who have difficulty maintaining stable breathing, which is indispensable for applying gating therapy, IMRT should be performed based on ITV. Based on the results, it was confirmed that tomotherapy is more suitable than other IMRT methods.

In this study, it was confirmed that the main dose error in a uniform target shape due to target motion in ITV-based tomotherapy treatment appears at both ends of the target SI direction. In most cases, the dose at the both ends of the target is lower than the dose calculated in the treatment plan, owing to the motion. This problem can be solved by an extension of the original ITV in the SI direction, considering the motion range. However, it is necessary to apply the method of expanding ITV only when there is no great risk considering the presence of OARs in the extended area of ITV.

## Conclusion

Among the various ITV-based IMRT methods, it was

confirmed by real dose measurements under motion conditions that the tomotherapy method has a relative advantage in the dosimetric similarity with the original plan compared to the general FB-IMRT or VMAT-type RapidArc methods in the case of a homogeneously shaped target.

When the target shape is relatively uniform and the motion is mainly in the SI direction during the tomotherapy treatment, the ITV could be slightly extended in the SI direction, considering the length of the motion range. This method could effectively reduce the dose error at both end regions of the original ITV.

### Conflicts of Interest

The author has nothing to disclose.

### Availability of Data and Materials

All relevant data are within the paper and its Supporting Information files.

### References

1. Nicolini G, Vanetti E, Clivio A, Fogliata A, Cozzi L. Pre-clinical evaluation of respiratory-gated delivery of volumetric modulated arc therapy with RapidArc. *Phys Med Biol.* 2010;55:N347-57.
2. Viel F, Lee R, Gete E, Duzenli C. Amplitude gated for a coached breathing approach in respiratory gated 10MV flattening filter-free VMAT delivery. *J Appl Clin Med Phys.* 2015;16:78-90.
3. Eccles C, Brock KK, Bissonnette JP, Hawkins M, Dawson LA. Reproducibility of liver position using active breathing coordinator for liver radiotherapy. *Int J Radiat Oncol Biol Phys.* 2006;64:751-9.
4. Brock J, McNair HA, Panakis N, Symonds-Tayler R, Evans PM, Brada M. The use of the Active Breathing Coordinator throughout radical non-small-cell lung cancer (NSCLC) radiotherapy. *Int J Radiat Oncol Biol Phys.* 2011;81:369-75.
5. Yakoumakis N, Winey B, Killoran J, et al. Using four-dimensional computed tomography images to optimize the internal target volume when using volume-modulated arc therapy to treat moving targets. *J Appl Clin Med Phys.* 2012;13:181-8.
6. Yeo SG, Kim ES. Efficient approach for determining four-dimensional computed tomography-based internal target volume in stereotactic radiotherapy of lung cancer. *Radiat Oncol J.* 2013;31:247-51.
7. Chen H, Wu A, Brandner ED, et al. Dosimetric evaluations of the interplay effect in respiratory-gated intensity-modulated radiation therapy. *Med Phys.* 2009;36:893-903.
8. Cheong KH, Kang SK, Lee M, et al. Evaluation of delivered monitor unit accuracy of gated step-and-shoot IMRT using a two-dimensional detector array. *Med Phys.* 2010;37:1146-51.
9. Kang H, Yorke ED, Yang J, Chui CS, Rosenzweig KE, Amols HI. Evaluation of tumor motion effects on dose distribution for hypofractionated intensity-modulated radiotherapy of non-small-cell lung cancer. *J Appl Clin Med Phys.* 2010;11:78-89.
10. Coleman L, Skourou C. Sensitivity of volumetric modulated arc therapy patient specific QA results to multileaf collimator errors and correlation to dose volume histogram based metrics. *Med Phys.* 2013;40:111715.
11. Riley C, Yang Y, Li T, Zhang Y, Heron DE, Huq MS. Dosimetric evaluation of the interplay effect in respiratory-gated RapidArc radiation therapy. *Med Phys.* 2014;41:011715.
12. Chaudhari SR, Goddu SM, Rangaraj D, et al. Dosimetric variances anticipated from breathing-induced tumor motion during tomotherapy treatment delivery. *Phys Med Biol.* 2009;54:2541-55.
13. Lu W. Real-time motion-adaptive delivery (MAD) using binary MLC: II. Rotational beam (tomotherapy) delivery. *Phys Med Biol.* 2008;53:6513-31.
14. Lu W, Chen M, Ruchala KJ, et al. Real-time motion-adaptive-optimization (MAO) in TomoTherapy. *Phys Med Biol.* 2009;54:4373-98.